


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100518\
 Data File : BG037155.D
 Acq On : 4 Oct 2018 14:56
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Sep 24 10:41:23 2018

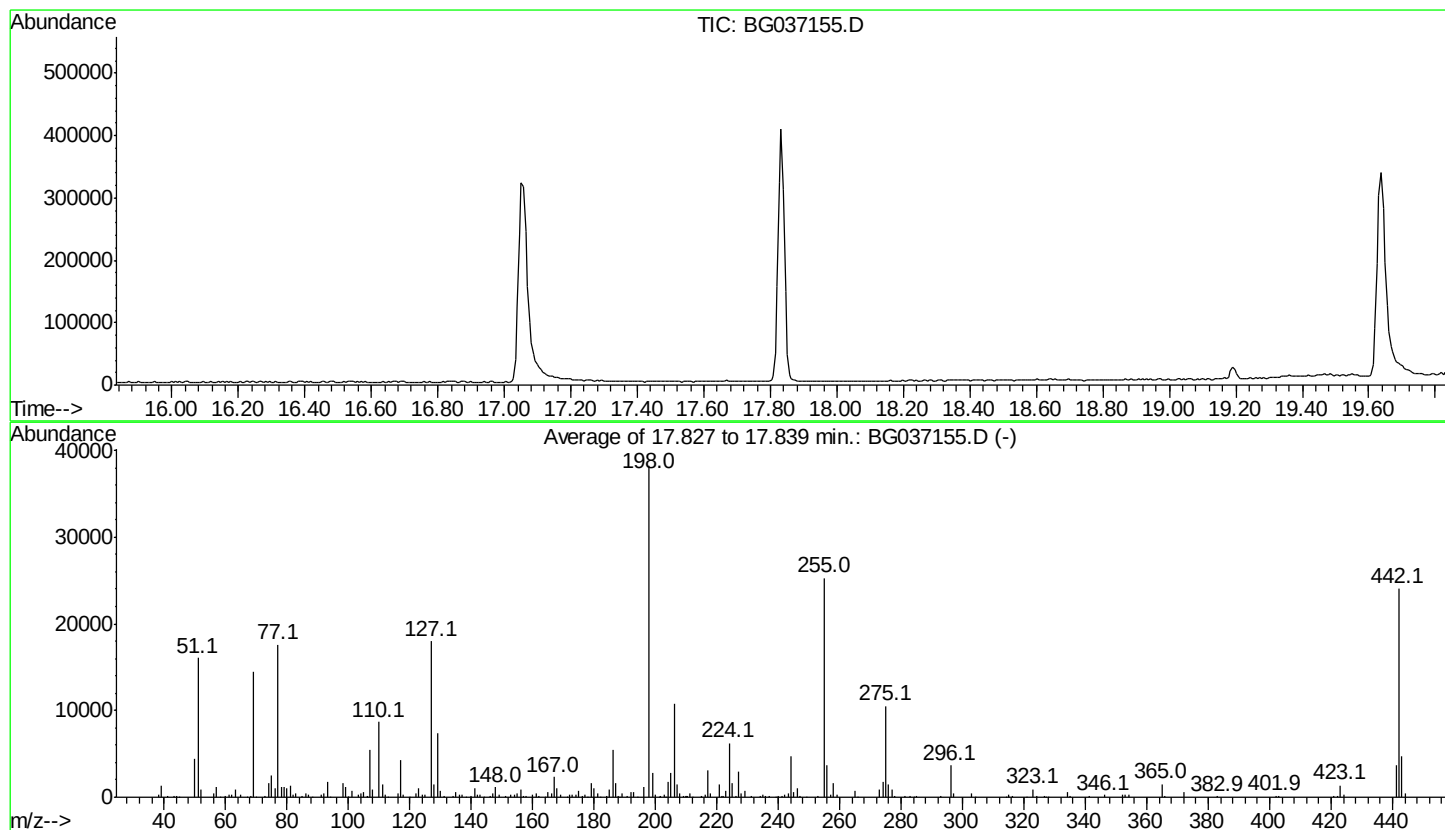

AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.0	16054	PASS
68	69	0.00	2	1.0	138	PASS
69	198	0.00	100	37.9	14502	PASS
70	69	0.00	2	0.3	50	PASS
127	198	10	80	46.9	17949	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	38248	PASS
199	198	5	9	7.5	2874	PASS
275	198	10	60	27.4	10492	PASS
365	198	1	100	4.0	1527	PASS
441	198	0.01	100	9.6	3667	PASS
442	198	50	100	62.8	24018	PASS
443	442	15	24	19.8	4747	PASS