

Data Path : Z:\HPCHEM1\BNA G\DATA\BG100615\
 Data File : BG019056.D
 Acq On : 6 Oct 2015 21:51
 Operator : UM/NP
 Sample : G3915-01
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 C03G2

Manual Integrations
 APPROVED

mmdadoda
 10/7/2015 4:49:46 PM

Quant Time: Oct 07 09:37:11 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG100415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Wed Oct 07 01:07:34 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.05	152	19091	20.00	ng/ul	0.00
18) Naphthalene-d8	10.85	136	84248	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.67	164	57807	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.42	188	152555	20.00	ng/ul	0.00
78) Chrysene-d12	21.69	240	197449	20.00	ng/ul	0.00
86) Perylene-d12	24.91	264	194224	20.00	ng/ul	-0.02

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.49	96	60m	0.14	ng/uL	0.00
5) Phenol-d5	7.20	99	4442	2.70	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.37	67	10752	10.10	ng/ul	0.00
9) 2-Chlorophenol-d4	7.58	132	10913	8.84	ng/ul	0.00
13) 4-Methylphenol-d8	8.75	113	8015	6.20	ng/ul	0.00
19) Nitrobenzene-d5	9.20	128	6650	10.44	ng/ul	0.00
22) 2-Nitrophenol-d4	9.93	143	7093	10.83	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.47	165	13560	10.34	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0	0.00	ng/ul	
44) Dimethylphthalate-d6	14.07	166	52746	11.57	ng/ul	0.00
47) Acenaphthylene-d8	14.36	160	58897	10.45	ng/ul	0.00
52) 4-Nitrophenol-d4	14.86	143	2721m	2.96	ng/ul	0.00
58) Fluorene-d10	15.66	176	46679	11.31	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.77	200	7699	9.30	ng/ul	0.00
71) Anthracene-d10	17.51	188	80760	11.24	ng/ul	0.00
79) Pyrene-d10	19.80	212	100852	11.03	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.69	264	106225	10.69	ng/ul	0.00

Target Compounds					Ovalue
45) Dimethylphthalate	14.12	163	43055	9.25 ng/ul	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG100615\
Data File : BG019056.D
Acq On : 6 Oct 2015 21:51
Operator : UM/NP
Sample : G3915-01
Misc :
ALS Vial : 7 Sample Multiplier: 1




Instrument :
BNA_G
ClientSampleId :
C03G2

Manual Integrations
APPROVED

mmdadoda
10/7/2015 4:49:46 PM

Quant Time: Oct 07 09:37:11 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG100415.M
Quant Title : SVOA CALIBRATION
QLast Update : Wed Oct 07 01:07:34 2015
Response via : Initial Calibration

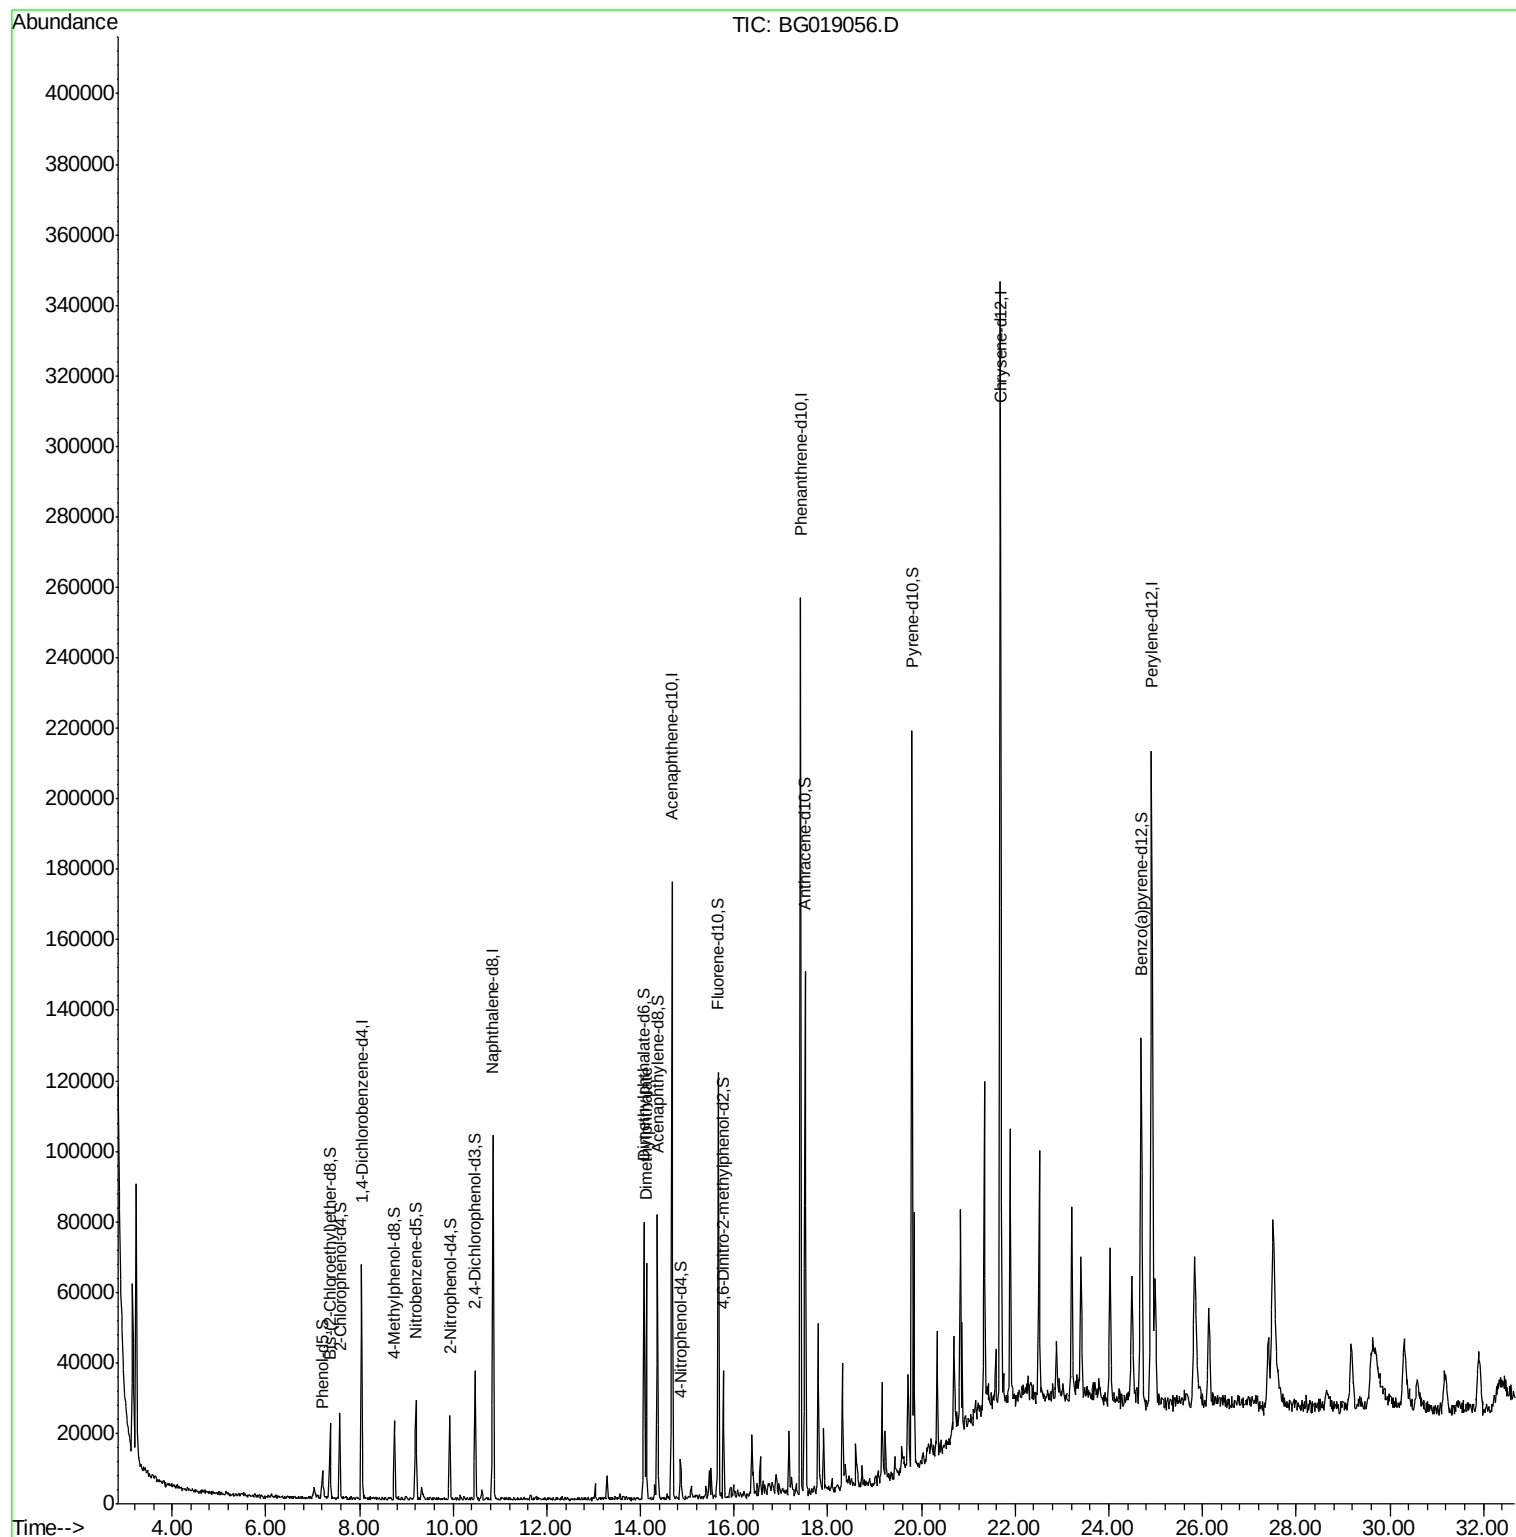

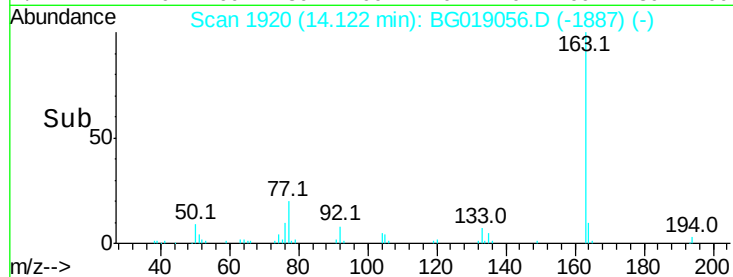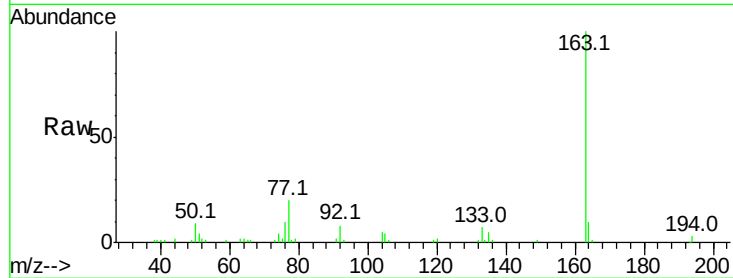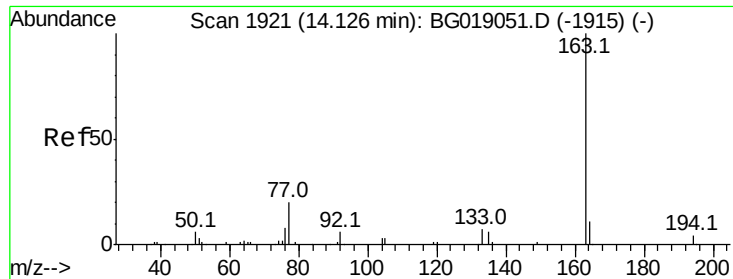

#45

Dimethylphthalate

Concen: 9.25 ng/ul

RT: 14.12 min Scan# 1920

Delta R.T. -0.00 min

Lab File: BG019056.D

Acq: 6 Oct 2015 21:51

Instrument :

BNA_G

ClientSampleId :

C03G2

Tot Ion:	163	Resp:	43055
Ion Ratio	Lower	Upper	
163	100		
194	3.4	3.3	4.9
164	9.7	8.1	12.1

Manual Integrations
APPROVED

mmdadoda
10/7/2015 4:49:46 PM

