


Data Path : Z:\HPCHEM1\BNA G\DATA\BG100615\
 Data File : BG019050.D
 Acq On : 6 Oct 2015 15:30
 Operator : UM/NP
 Sample : DFTPP62
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP62

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG100415.M
 Title : SVOA CALIBRATION
 Last Update : Wed Oct 07 12:49:07 2015

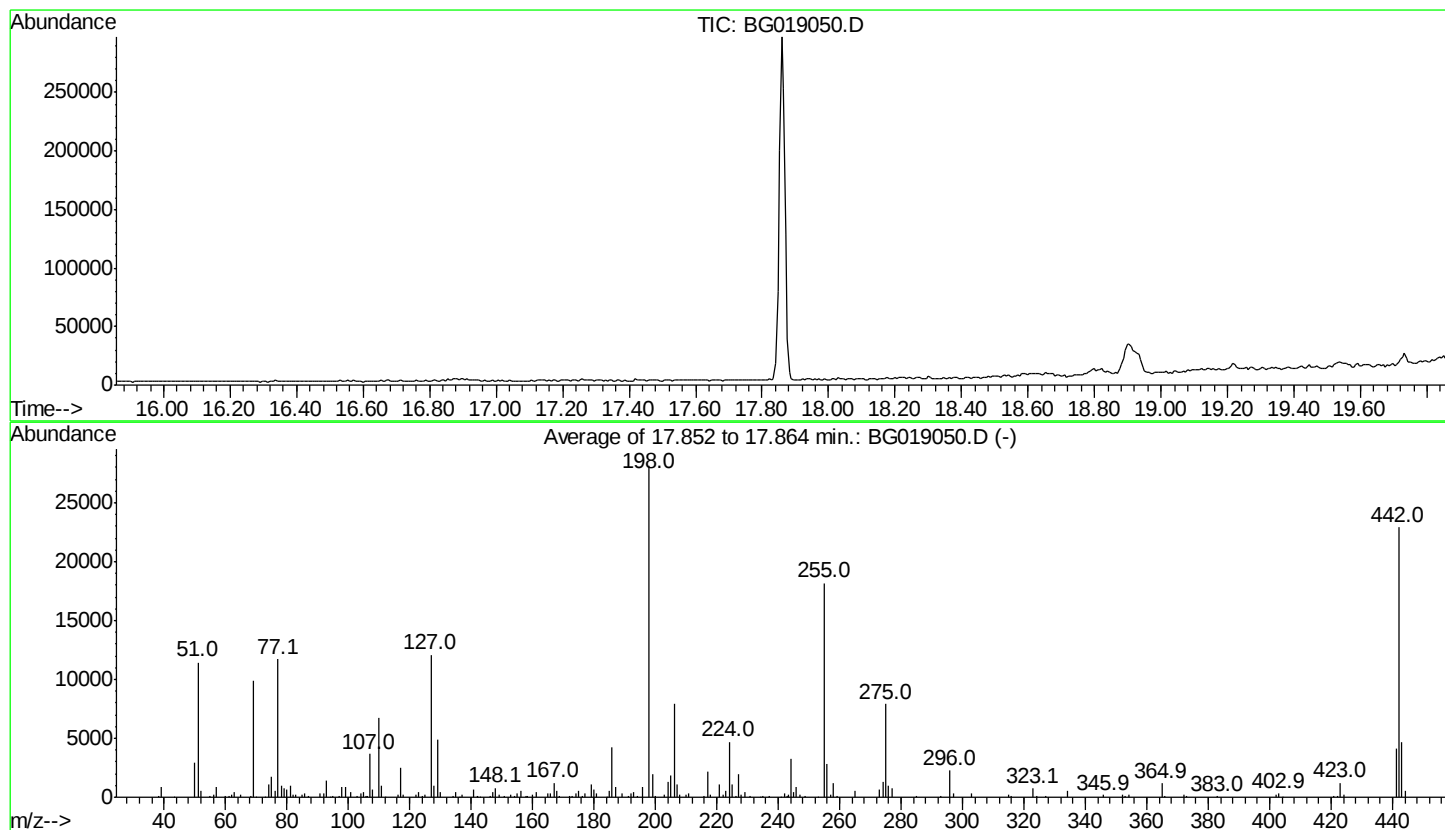

AutoFind: Scans 2555, 2556, 2557; Background Corrected with Scan 2550

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.6	11444	PASS
68	69	0.00	2	0.7	71	PASS
69	198	0.00	100	35.1	9878	PASS
70	69	0.00	2	0.5	50	PASS
127	198	10	80	43.0	12112	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	28160	PASS
199	198	5	9	7.1	1994	PASS
275	198	10	60	28.1	7902	PASS
365	198	1	100	4.2	1186	PASS
441	442	0.01	24	17.8	4083	PASS
442	198	50	100	81.3	22905	PASS
443	442	15	24	20.2	4631	PASS

Scan 2550 (17.823 min): BG019050.D
DFTPP62

m/z	Abundance
40.00	451.0
41.10	299.0
43.10	334.0
44.00	795.0
45.10	156.0
49.00	833.0
51.00	273.0
55.10	187.0
56.10	160.0
57.10	158.0
69.10	200.0
73.00	151.0
83.90	512.0
86.10	210.0
207.00	239.0

Instrument :
BNA_G
ClientSampleId :
DFTPP62

m/z	Abundance
39.10	885.0
40.00	258.0
41.10	285.0
43.10	349.0
44.00	848.0
49.10	966.0
50.10	2709.0
51.10	11278.0
52.10	537.0
55.00	271.0
56.00	379.0
57.10	962.0
60.10	161.0
61.00	158.0
62.00	302.0
63.00	384.0
65.10	203.0
69.00	8992.0
70.10	152.0
73.10	249.0
74.00	1225.0
75.00	1484.0
76.10	624.0
77.10	10669.0
78.10	997.0
79.00	744.0
80.10	654.0
81.00	871.0
83.00	317.0
83.90	401.0
85.00	255.0
86.00	436.0
91.00	256.0
92.00	277.0
93.00	1197.0
98.00	809.0
99.00	731.0
101.00	434.0
104.00	340.0
105.00	299.0
107.00	3043.0
108.10	797.0
110.00	5899.0
111.00	821.0
112.00	161.0
116.00	206.0
117.00	2155.0
118.00	259.0
121.90	235.0
123.00	367.0
124.00	185.0
125.10	186.0
127.00	10700.0
128.00	804.0
129.00	4138.0
130.00	418.0
134.90	371.0
136.10	155.0
137.00	273.0
141.00	610.0
141.90	162.0
147.00	382.0
148.10	699.0
148.90	179.0
155.00	330.0
156.10	490.0
158.00	229.0
159.90	159.0
161.00	292.0
164.90	203.0
166.00	204.0
167.00	1006.0
168.00	577.0
168.90	174.0
171.90	155.0
173.00	195.0
174.00	289.0
175.10	407.0
177.00	244.0
179.00	882.0
180.00	444.0
181.00	260.0
185.00	472.0
186.00	3437.0
187.00	827.0
188.90	308.0
191.10	202.0
192.00	234.0
193.10	380.0
196.00	646.0
198.00	23328.0
199.00	1782.0

Instrument :
BNA_G
ClientSampleId :
DFTPP62

204.00	1018.0
205.00	1451.0
206.10	6742.0
207.10	1217.0
208.00	242.0
210.00	151.0
211.00	277.0
216.00	169.0
217.00	1702.0
217.90	155.0
221.00	802.0
223.00	524.0
224.00	3751.0
225.00	1204.0
227.00	1568.0
229.00	336.0
241.00	163.0
242.00	283.0
243.10	233.0
244.00	2645.0
245.00	335.0
246.00	673.0
246.90	243.0
255.00	14110.0
256.00	1971.0
256.90	218.0
258.00	936.0
259.00	204.0
265.10	428.0
272.90	435.0
274.00	828.0
275.00	6027.0
276.00	723.0
277.00	448.0
296.00	1716.0
297.00	219.0
303.10	200.0
315.00	199.0
323.00	472.0
334.00	293.0
345.90	178.0
351.90	184.0
364.90	536.0
402.00	186.0
403.10	204.0
423.00	562.0
441.10	2172.0
442.00	13469.0
443.00	2775.0
444.00	304.0

Instrument :
BNA_G
ClientSampleId :
DFTPP62

m/z	Abundance
38.10	283.0
39.10	1152.0
40.00	377.0
41.10	280.0
43.10	404.0
44.10	800.0
45.00	214.0
49.00	765.0
50.10	3484.0
51.10	13758.0
52.10	581.0
55.10	295.0
56.10	411.0
57.10	1135.0
61.10	222.0
62.00	214.0
63.10	484.0
65.00	179.0
69.00	12344.0
73.00	169.0
74.10	1130.0
75.00	2291.0
76.10	648.0
77.10	14241.0
78.10	1340.0
79.00	872.0
80.00	750.0
81.00	1263.0
82.10	318.0
83.00	208.0
84.00	458.0
85.10	170.0
86.00	669.0
87.10	285.0
91.00	375.0
92.00	354.0
93.00	1661.0
94.00	173.0
95.20	195.0
97.00	186.0
98.00	1132.0
99.00	992.0
101.00	532.0
103.00	231.0
104.10	377.0
105.00	553.0
105.90	188.0
107.00	4369.0
108.00	809.0
110.00	7992.0
111.00	1153.0
116.00	277.0
117.00	2899.0
118.00	206.0
122.00	299.0
123.00	422.0
124.00	197.0
125.00	315.0
127.00	13778.0
128.00	1089.0
129.00	5369.0
130.00	610.0
133.90	171.0
135.00	429.0
141.00	703.0
142.10	178.0
142.90	173.0
147.00	574.0
148.00	923.0
149.00	396.0
151.00	183.0
153.00	329.0
154.00	296.0
155.00	485.0
156.00	535.0
157.80	193.0
159.80	226.0
161.10	475.0
165.00	447.0
166.00	337.0
167.00	1335.0
168.00	620.0
172.00	151.0
173.00	251.0
174.10	473.0
175.00	768.0
176.10	216.0
177.00	442.0
179.00	1542.0
180.00	749.0
181.00	402.0
184.00	151.0

Instrument :
BNA_G
ClientSampleId :
DFTPP62

185.10	657.0
186.00	5132.0
187.10	1026.0
189.00	245.0
191.00	231.0
192.00	459.0
193.00	516.0
194.00	197.0
196.00	950.0
198.00	33064.0
199.00	2326.0
199.90	228.0
202.90	244.0
204.00	1355.0
205.00	2393.0
206.00	9625.0
207.00	1237.0
208.00	259.0
210.00	150.0
210.90	407.0
216.00	227.0
217.00	2833.0
218.00	412.0
221.00	1222.0
222.00	375.0
223.00	581.0
224.00	5603.0
225.00	1206.0
226.20	230.0
227.00	2252.0
228.00	278.0
229.00	487.0
231.00	291.0
234.00	151.0
235.00	223.0
237.00	271.0
242.00	269.0
243.10	328.0
244.00	3971.0
245.00	549.0
246.00	1006.0
247.00	239.0
248.90	204.0
253.00	151.0
255.00	21456.0
256.00	3560.0
257.00	209.0
258.00	1435.0
265.00	642.0
273.00	612.0
274.00	1867.0
275.00	8923.0
276.00	1207.0
277.00	879.0
293.00	237.0
296.00	2609.0
297.10	328.0
303.10	349.0
314.90	316.0
316.00	284.0
323.00	895.0
324.00	178.0
327.00	208.0
334.00	698.0
345.90	176.0
352.00	280.0
353.10	173.0
354.10	293.0
365.00	1400.0
365.90	192.0
372.00	368.0
402.00	243.0
402.90	363.0
421.00	198.0
422.00	151.0
423.00	1551.0
424.00	279.0
441.00	4788.0
442.00	26912.0
443.00	5456.0
444.00	629.0

Instrument :
BNA_G
ClientSampleId :
DFTPP62

m/z	Abundance
39.10	740.0
40.00	409.0
41.10	212.0
43.10	375.0
44.10	719.0
49.00	704.0
50.10	2715.0
51.10	10116.0
52.00	482.0
55.10	291.0
56.10	356.0
57.00	1019.0
60.10	215.0
62.10	196.0
63.10	362.0
65.10	185.0
68.10	214.0
69.00	8900.0
73.10	163.0
74.10	834.0
75.00	1459.0
76.00	420.0
77.10	10283.0
78.00	612.0
79.00	701.0
80.00	649.0
81.00	815.0
82.00	346.0
83.00	283.0
84.00	421.0
84.90	182.0
86.00	502.0
91.00	318.0
92.00	213.0
93.00	1312.0
95.10	164.0
98.00	804.0
99.00	933.0
101.00	501.0
104.00	287.0
105.00	436.0
106.10	209.0
107.00	3641.0
108.00	428.0
110.00	6314.0
111.00	944.0
116.10	243.0
117.00	2591.0
117.90	152.0
121.90	204.0
123.00	398.0
125.00	223.0
127.00	11860.0
128.00	1145.0
129.00	5235.0
129.90	312.0
134.00	159.0
135.10	473.0
137.10	238.0
141.00	511.0
142.00	199.0
146.10	198.0
147.00	442.0
148.00	807.0
148.90	161.0
153.00	276.0
154.00	159.0
155.10	268.0
156.00	472.0
158.10	208.0
159.90	173.0
161.00	469.0
165.00	300.0
165.90	295.0
167.00	1308.0
168.00	591.0
172.00	184.0
173.90	293.0
175.10	447.0
176.00	155.0
177.10	209.0
178.90	994.0
180.10	642.0
181.00	454.0
185.00	506.0
186.00	4153.0
187.00	904.0
188.90	284.0
191.90	305.0
193.00	392.0
196.00	877.0
198.00	28088.0

Instrument :
BNA_G
ClientSampleId :
DFTPP62

199.00	1874.0
203.00	400.0
204.00	1422.0
205.00	1728.0
206.00	7485.0
207.10	1448.0
208.00	291.0
210.00	214.0
211.00	341.0
217.00	2014.0
218.00	198.0
221.00	1185.0
222.00	293.0
222.90	597.0
224.00	4679.0
225.00	869.0
227.00	1991.0
228.00	407.0
228.90	458.0
231.00	189.0
237.00	210.0
242.00	288.0
242.80	200.0
244.00	3266.0
245.00	485.0
245.90	930.0
246.90	186.0
255.00	18936.0
256.00	3007.0
256.90	160.0
257.90	1197.0
259.00	179.0
264.90	649.0
273.00	825.0
274.00	1318.0
275.00	8757.0
276.00	1091.0
277.00	854.0
285.00	209.0
292.90	195.0
296.00	2476.0
297.00	417.0
303.00	285.0
315.00	271.0
323.10	832.0
324.00	197.0
327.00	158.0
334.00	581.0
345.90	254.0
352.00	286.0
352.90	163.0
354.00	262.0
365.00	1622.0
372.00	440.0
372.90	213.0
383.00	233.0
402.00	189.0
402.90	286.0
404.10	161.0
420.90	266.0
421.90	178.0
423.00	1592.0
424.10	345.0
441.00	5291.0
442.00	28336.0
443.00	5663.0
444.00	599.0

Instrument :
BNA_G
ClientSampleId :
DFTPP62