
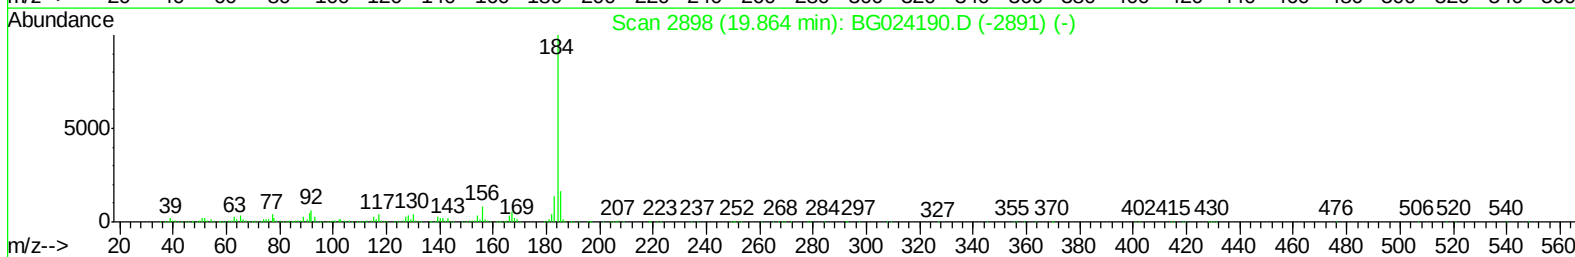
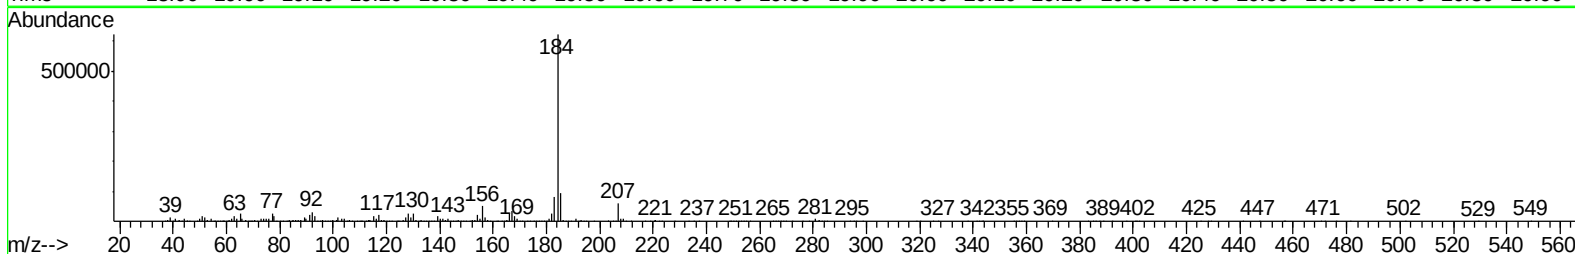


Data Path : Z:\HPCHEM1\BNA G\DATA\BG100616\
Data File : BG024186.D
Acq On : 6 Oct 2016 1:23
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 06 13:30:38 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG100616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 06 11:45:13 2016
Response via : Initial Calibration

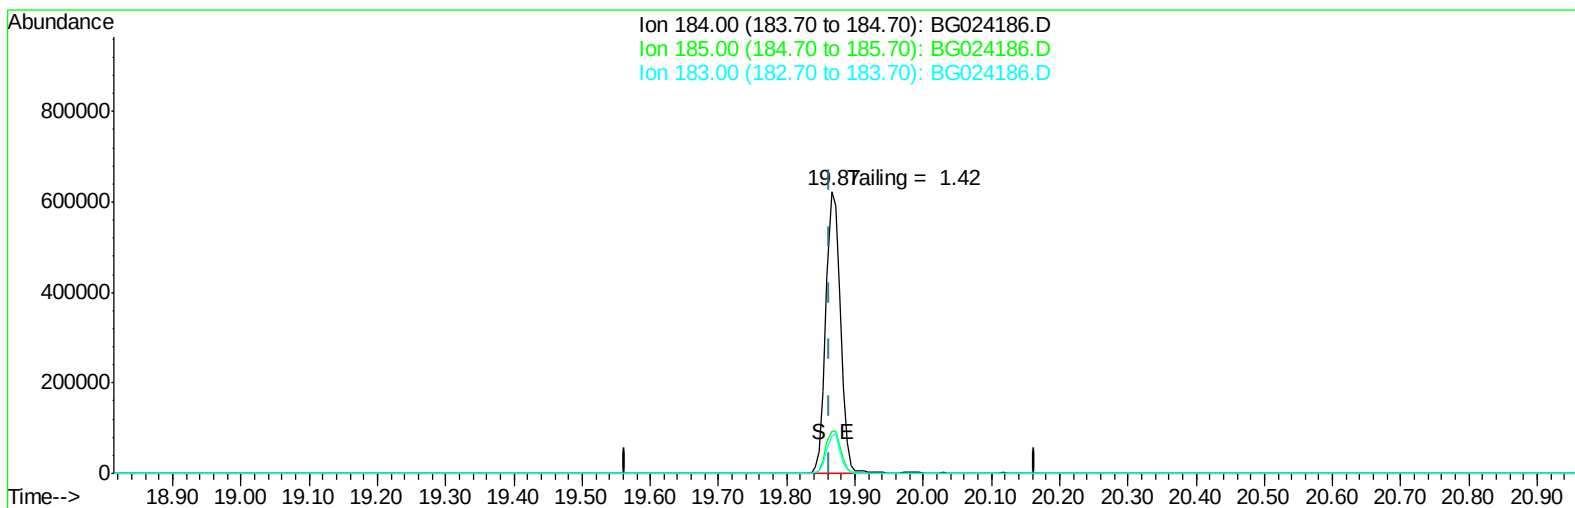

TIC: BG024186.D

(76) Benzidine




19.865min (+0.001) 685953.12ng

response 917275

Ion	Exp%	Act%
184.00	100	100
185.00	16.30	15.00
183.00	13.80	13.01
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\DATA\BG100616\
Data File : BG024186.D
Acq On : 6 Oct 2016 1:23
Operator : UM/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 06 13:30:38 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG100616.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 06 11:45:13 2016
Response via : Initial Calibration

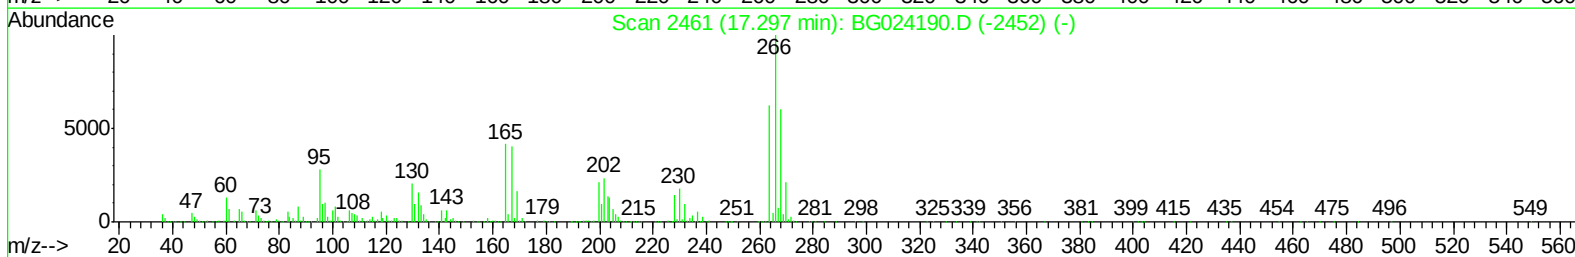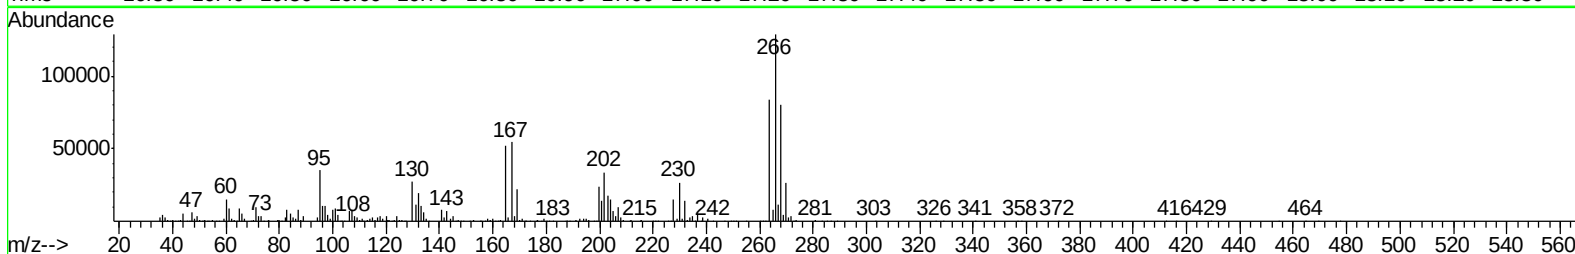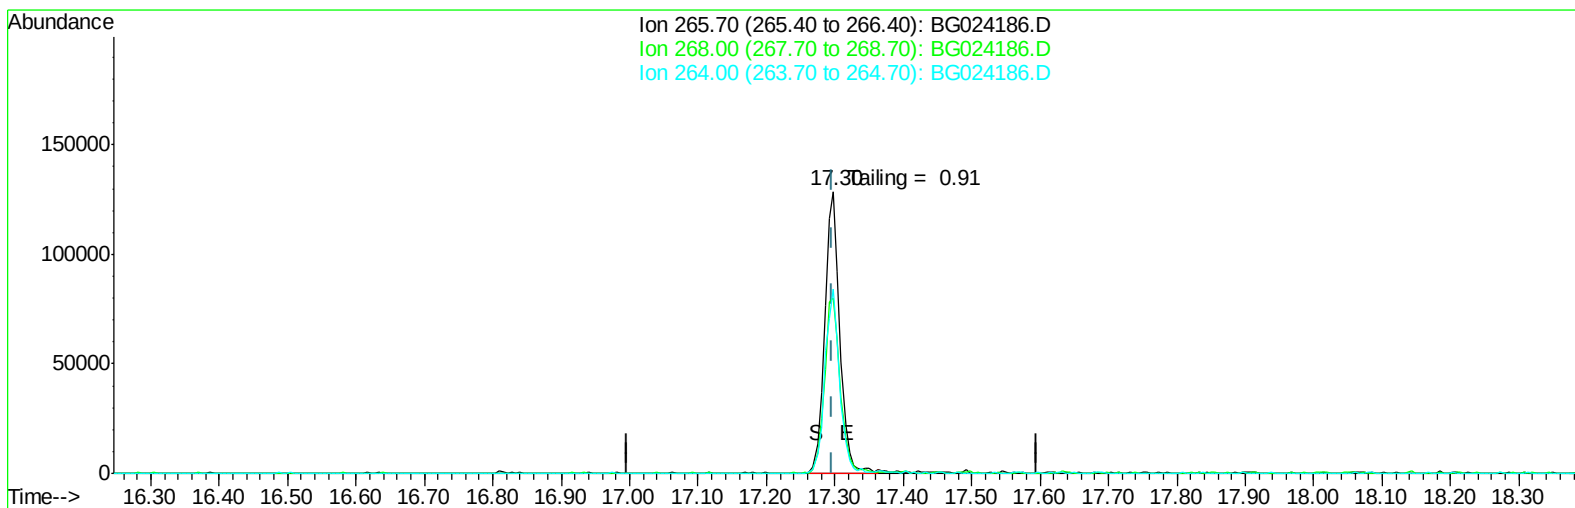

TIC: BG024186.D

(69) Pentachlorophenol (C)

17.298min (+0.001) 230260.61ng

response 200000

Ion	Exp%	Act%
265.70	100	100
268.00	60.70	62.27
264.00	62.60	65.47
0.00	0.00	0.00