


Data Path : Z:\HPCHEM1\BNA G\DATA\BG100616\
 Data File : BG024186.D
 Acq On : 6 Oct 2016 1:23
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG100616.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 06 11:45:13 2016

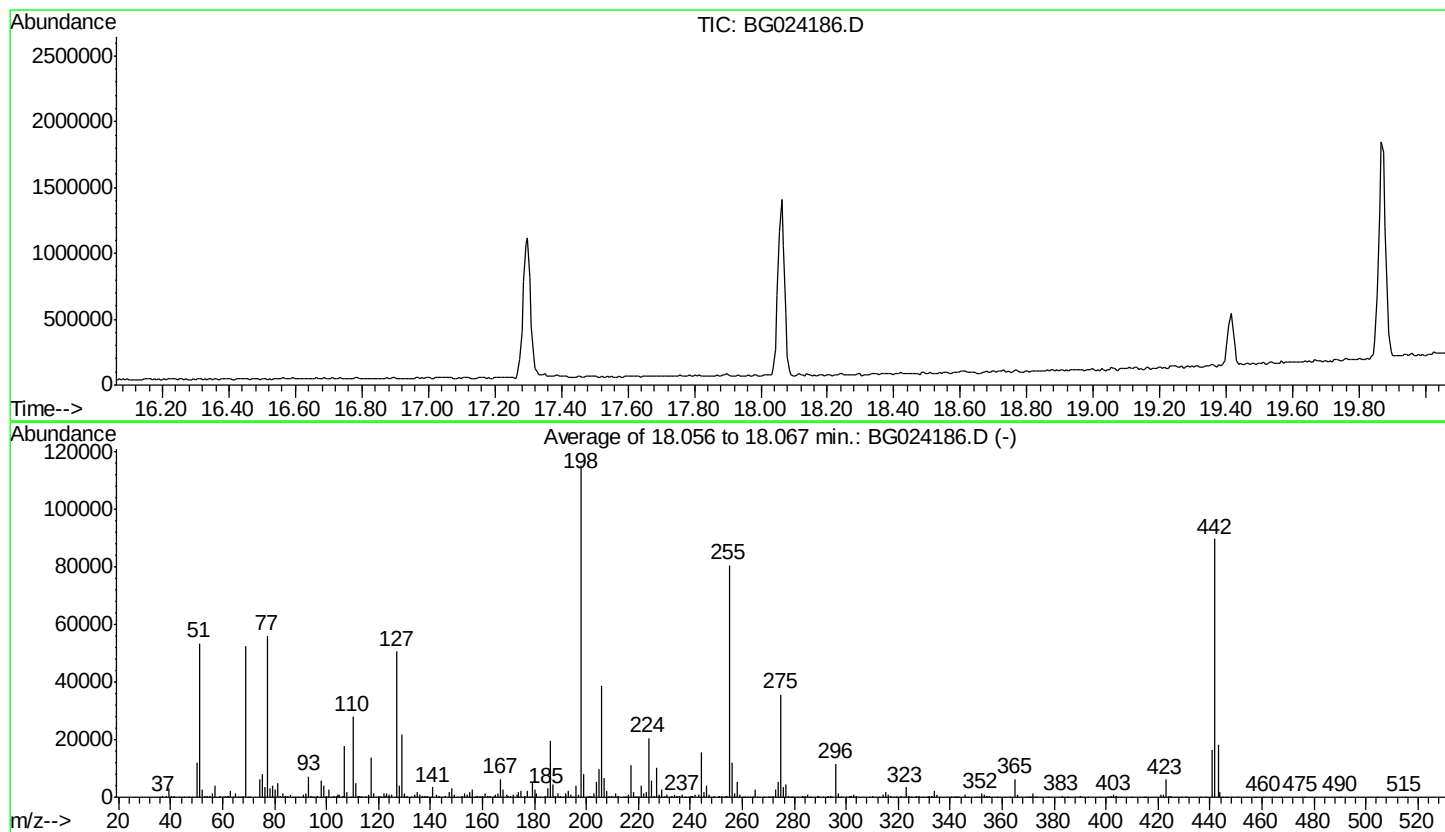

AutoFind: Scans 2590, 2591, 2592; Background Corrected with Scan 2583

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.4	53513	PASS
68	69	0.00	2	0.7	358	PASS
69	198	0.00	100	45.7	52693	PASS
70	69	0.00	2	0.4	231	PASS
127	198	10	80	44.0	50733	PASS
197	198	0.00	2	0.7	848	PASS
198	198	100	100	100.0	115328	PASS
199	198	5	9	6.8	7842	PASS
275	198	10	60	30.9	35693	PASS
365	198	1	100	5.5	6368	PASS
441	442	0.01	24	18.4	16506	PASS
442	198	50	100	77.9	89880	PASS
443	442	15	24	20.1	18054	PASS