

Data Path : Z:\HPCHEM1\BNA G\Data\BG100716\RAW\
 Data File : BG024203.D
 Acq On : 6 Oct 2016 17:41
 Operator : UM/SJ
 Sample : H5080-03
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDNA4

Quant Time: Oct 07 09:22:52 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 07 06:34:32 2016
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.303	152	137626	20.00	ng/ul	0.00
18) Naphthalene-d8	11.129	136	605514	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.913	164	484036	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.657	188	1050235	20.00	ng/ul	0.00
75) Chrysene-d12	21.958	240	1138868	20.00	ng/ul	0.00
83) Perylene-d12	25.412	264	1136199	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.655	96	7537	2.60	ng/uL	0.00
5) Phenol-d5	7.428	99	234088	18.23	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	7.616	67	172377	19.86	ng/ul	0.00
9) 2-Chlorophenol-d4	7.821	132	173390	19.61	ng/ul	0.00
13) 4-Methylphenol-d8	8.985	113	183720	17.70	ng/ul	0.00
19) Nitrobenzene-d5	9.478	128	89129	20.74	ng/ul	0.00
22) 2-Nitrophenol-d4	10.201	143	97267	20.23	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.735	165	183926	17.57	ng/ul	0.00
29) 4-Chloroaniline-d4	11.258	131	206639	18.78	ng/ul	0.00
43) Dimethylphthalate-d6	14.314	166	669968	19.82	ng/ul	0.00
46) Acenaphthylene-d8	14.613	160	777784	20.09	ng/ul	0.00
51) 4-Nitrophenol-d4	15.072	143	101708	16.97	ng/ul	0.00
57) Fluorene-d10	15.900	176	649235	20.32	ng/ul	0.00
62) 4,6-Dinitro-2-methylph...	16.000	200	96147	15.23	ng/ul	0.00
70) Anthracene-d10	17.757	188	993821	20.95	ng/ul	0.00
76) Pyrene-d10	20.025	212	1131239	21.28	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.171	264	1025777	20.07	ng/ul	0.00
Target Compounds						
44) Dimethylphthalate	14.355	163	538823	16.26	ng/ul	Ovalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\Data\BG100716\RAW\
Data File : BG024203.D
Acq On : 6 Oct 2016 17:41
Operator : UM/SJ
Sample : H5080-03
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDNA4

Quant Time: Oct 07 09:22:52 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 07 06:34:32 2016
Response via : Initial Calibration

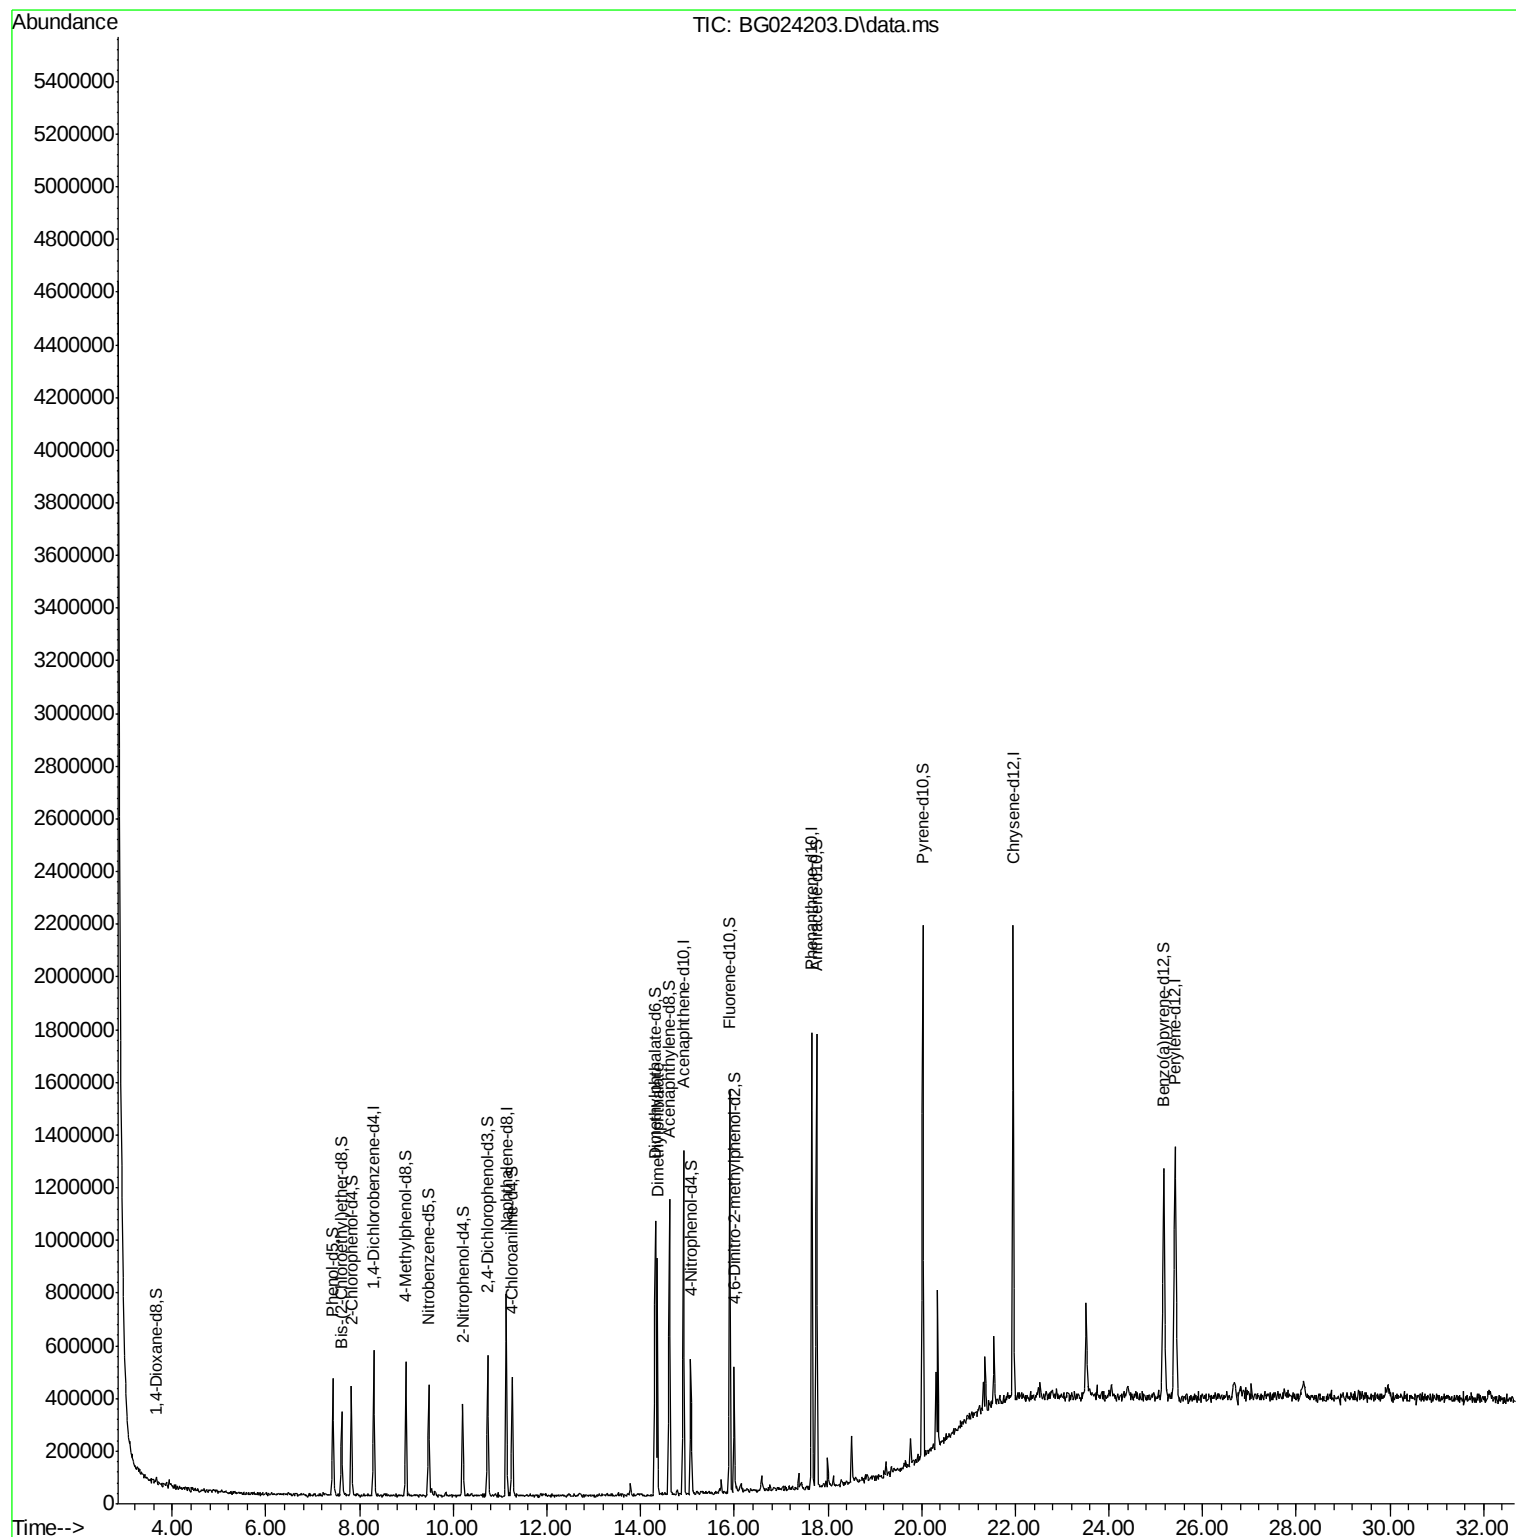

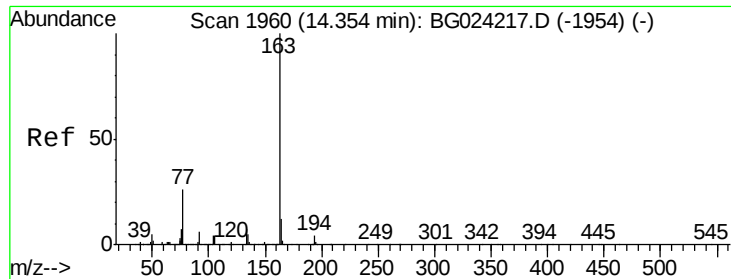

#44

Dimethylphthalate

Concen: 16.26 ng/ul

RT: 14.355 min Scan# 19

Delta R.T. 0.000 min

Lab File: BG024203.D

Acq: 6 Oct 2016 17:41

Instrument :

BNA_G

ClientSampleId :

BDNA4

Tot Ion:163 Resp: 538823

Ion Ratio Lower Upper

163 100

194 5.1 3.4 5.2

164 9.7 8.8 13.2

