

Data Path : Z:\HPCHEM1\BNA G\Data\BG100716\RAW\
 Data File : BG024204.D
 Acq On : 6 Oct 2016 18:20
 Operator : UM/SJ
 Sample : H5080-06
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDNA6

Quant Time: Oct 07 09:24:20 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 07 06:34:32 2016
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.302	152	160424	20.00	ng/ul	0.00
18) Naphthalene-d8	11.134	136	672013	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.918	164	537281	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.755	188	1656922	20.00	ng/ul	0.10
75) Chrysene-d12	21.956	240	1283336	20.00	ng/ul	0.00
83) Perylene-d12	25.411	264	1297137	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.654	96	14244	4.22	ng/uL	0.00
5) Phenol-d5	7.426	99	390692	26.10	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	7.614	67	275496	27.23	ng/ul	0.00
9) 2-Chlorophenol-d4	7.826	132	289350	28.07	ng/ul	0.00
13) 4-Methylphenol-d8	8.989	113	334522	27.65	ng/ul	0.00
19) Nitrobenzene-d5	9.477	128	136505	28.62	ng/ul	0.00
22) 2-Nitrophenol-d4	10.194	143	158766	29.76	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.734	165	320028	27.54	ng/ul	0.00
29) 4-Chloroaniline-d4	11.257	131	419137	34.33	ng/ul	0.00
43) Dimethylphthalate-d6	14.312	166	1143799	30.49	ng/ul	0.00
46) Acenaphthylene-d8	14.612	160	1330398	30.96	ng/ul	0.00
51) 4-Nitrophenol-d4	15.076	143	188532	28.34	ng/ul	0.00
57) Fluorene-d10	15.899	176	1093239	30.82	ng/ul	0.00
62) 4,6-Dinitro-2-methylph...	16.087	200	218	0.02	ng/ul	0.09
70) Anthracene-d10	17.861	188	1812	0.02	ng/ul	0.10
76) Pyrene-d10	20.023	212	1876579	31.33	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.176	264	1889351	32.37	ng/ul	0.01
Target Compounds						
44) Dimethylphthalate	14.359	163	744997	20.25	ng/ul	Ovalue 97




(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\Data\BG100716\RAW\
Data File : BG024204.D
Acq On : 6 Oct 2016 18:20
Operator : UM/SJ
Sample : H5080-06
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDNA6

Quant Time: Oct 07 09:24:20 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 07 06:34:32 2016
Response via : Initial Calibration

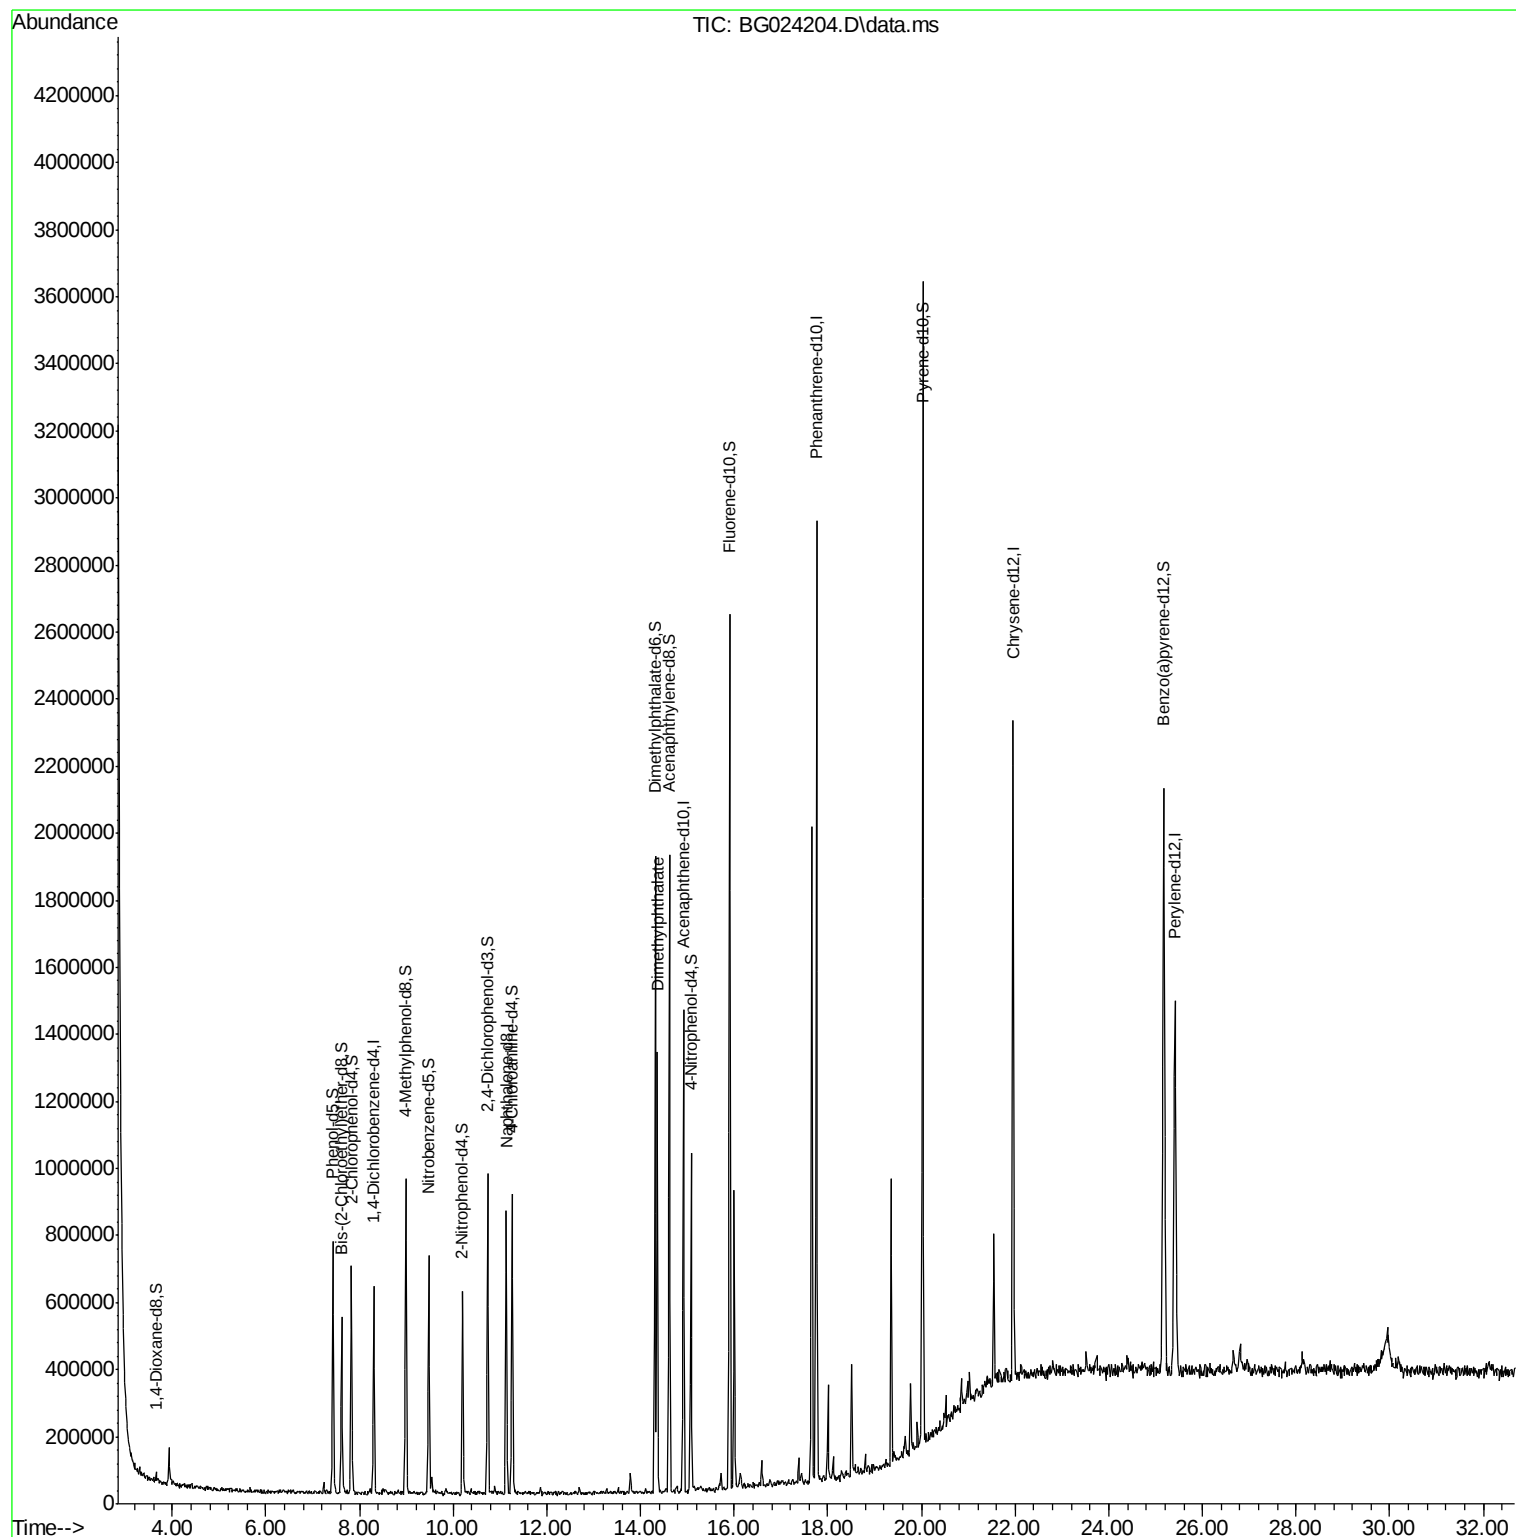

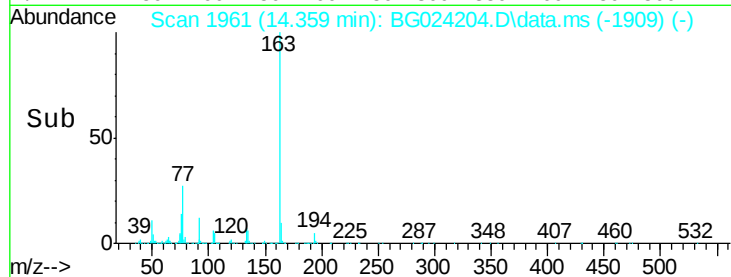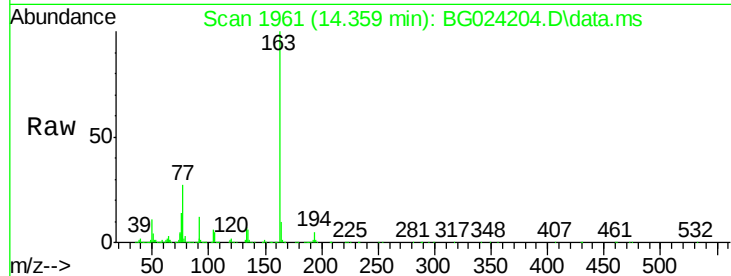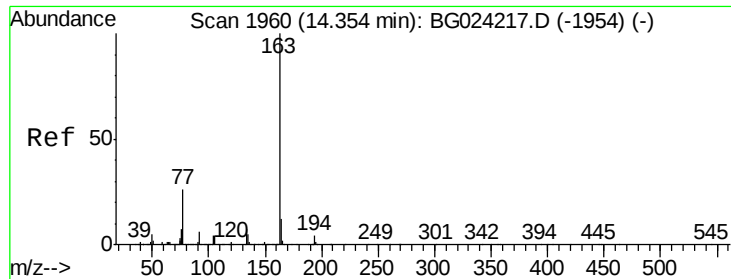

#44

Dimethylphthalate

Concen: 20.25 ng/ul

RT: 14.359 min Scan# 19

Delta R.T. 0.005 min

Lab File: BG024204.D

Acq: 6 Oct 2016 18:20

Instrument :

BNA_G

ClientSampleId :

BDNA6

Tot Ion:163 Resp: 744997

Ion Ratio Lower Upper

163 100

194 4.9 3.4 5.2

164 9.8 8.8 13.2

