

Data Path : Z:\HPCHEM1\BNA G\Data\BG100716\RAW\
 Data File : BG024207.D
 Acq On : 6 Oct 2016 20:15
 Operator : UM/SJ
 Sample : H5082-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDPH2

Quant Time: Oct 07 09:25:43 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 07 06:34:32 2016
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.298	152	150737	20.00	ng/ul	0.00
18) Naphthalene-d8	11.130	136	635975	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.914	164	513451	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.752	188	1060396	20.00	ng/ul	0.10
75) Chrysene-d12	21.959	240	1210529	20.00	ng/ul	0.00
83) Perylene-d12	25.413	264	1226728	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.656	96	9910	3.12	ng/uL	0.00
5) Phenol-d5	7.429	99	236285	16.80	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	7.611	67	171056	17.99	ng/ul	0.00
9) 2-Chlorophenol-d4	7.822	132	173019	17.87	ng/ul	0.00
13) 4-Methylphenol-d8	8.986	113	205399	18.07	ng/ul	0.00
19) Nitrobenzene-d5	9.473	128	83471	18.49	ng/ul	0.00
22) 2-Nitrophenol-d4	10.202	143	97353	19.28	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.731	165	192224	17.48	ng/ul	0.00
29) 4-Chloroaniline-d4	11.259	131	242824	21.02	ng/ul	0.00
43) Dimethylphthalate-d6	14.309	166	712761	19.88	ng/ul	0.00
46) Acenaphthylene-d8	14.614	160	824418	20.08	ng/ul	0.00
51) 4-Nitrophenol-d4	15.073	143	97028	15.26	ng/ul	0.00
57) Fluorene-d10	15.901	176	674057	19.89	ng/ul	0.00
62) 4,6-Dinitro-2-methylph...	16.095	200	152	0.02	ng/ul	0.10
70) Anthracene-d10	17.711	188	1128	0.02	ng/ul	-0.05
76) Pyrene-d10	20.020	212	1206802	21.36	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.167	264	1166468	21.13	ng/ul	0.00
Target Compounds						
44) Dimethylphthalate	14.356	163	589617	16.77	ng/ul	Ovalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\Data\BG100716\RAW\
Data File : BG024207.D
Acq On : 6 Oct 2016 20:15
Operator : UM/SJ
Sample : H5082-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDPH2

Quant Time: Oct 07 09:25:43 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 07 06:34:32 2016
Response via : Initial Calibration

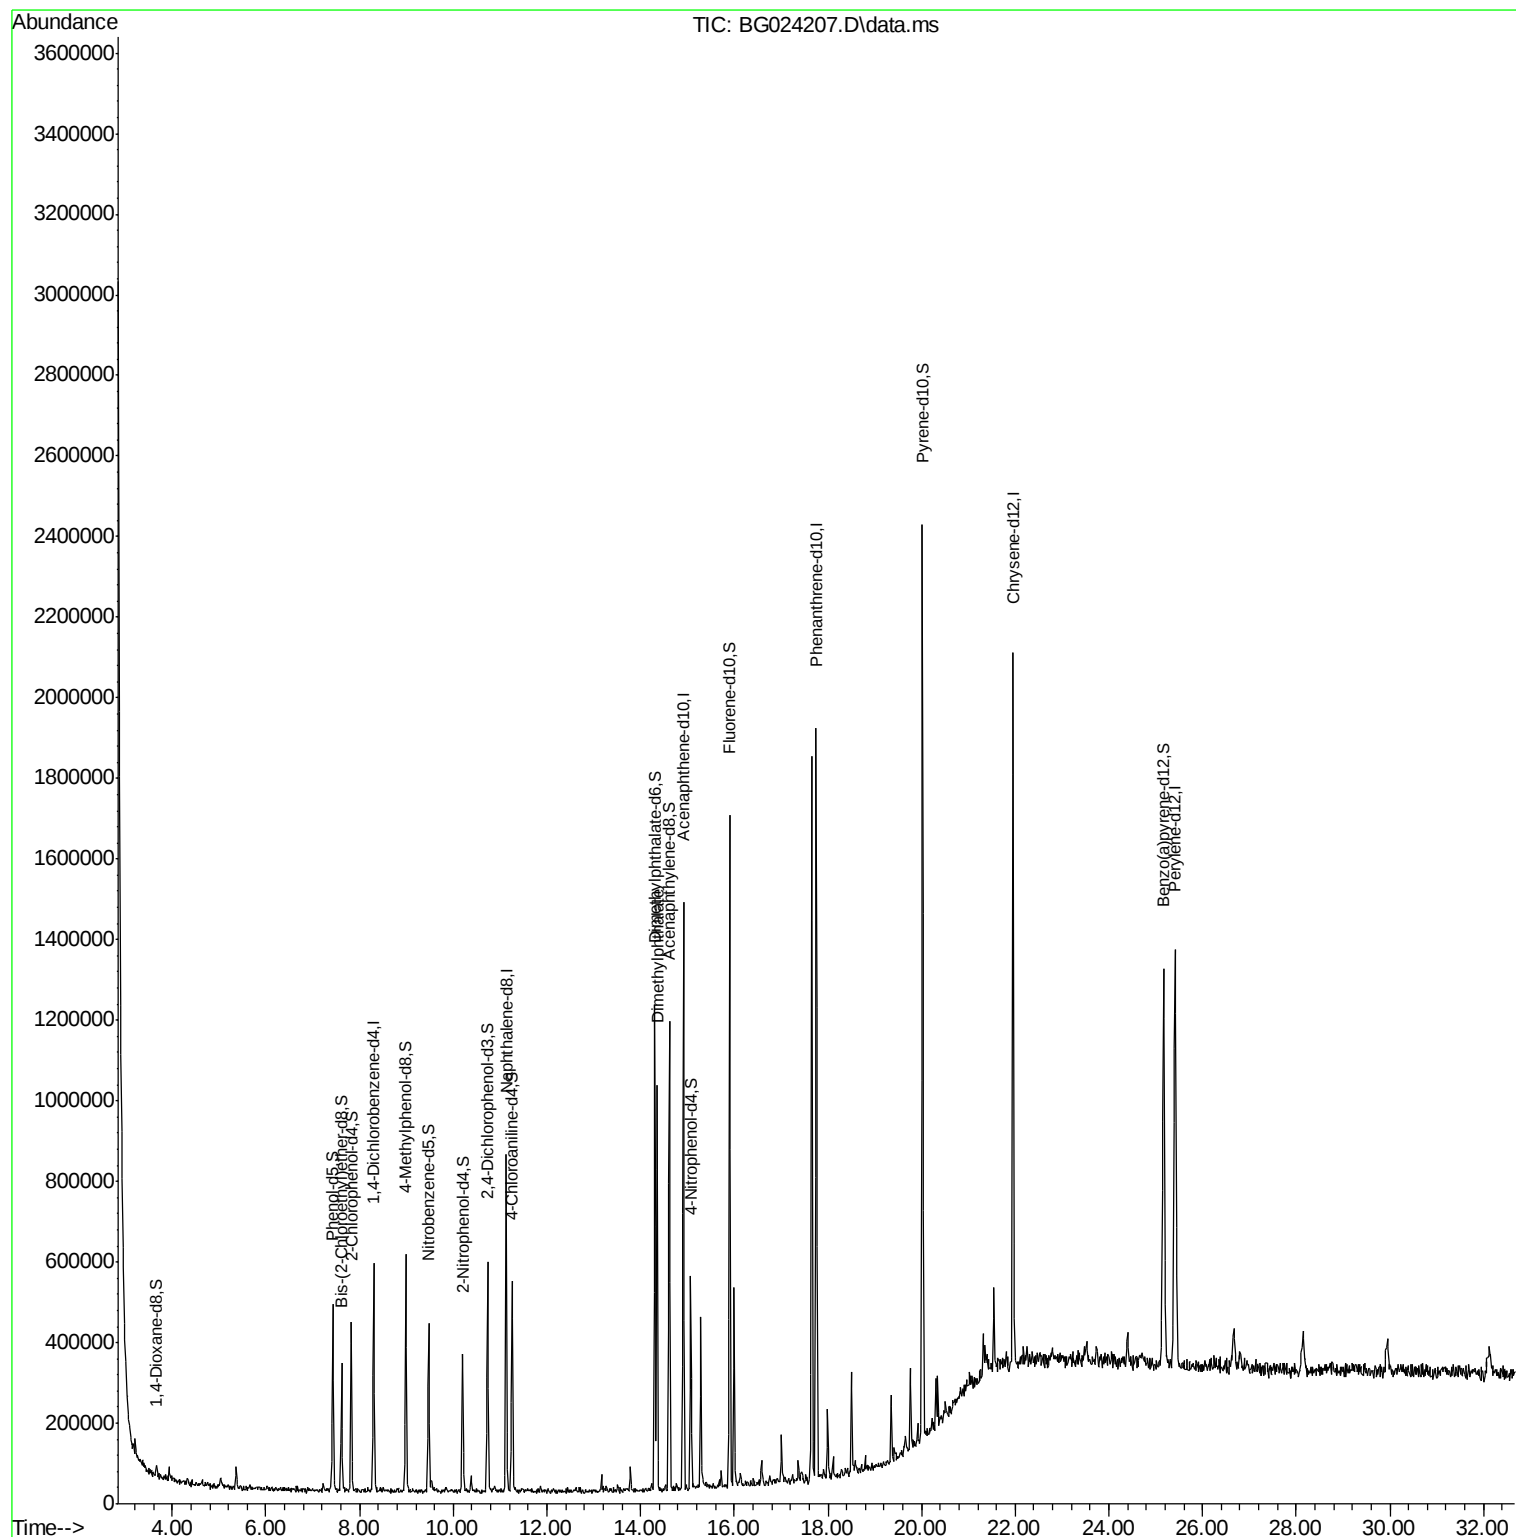

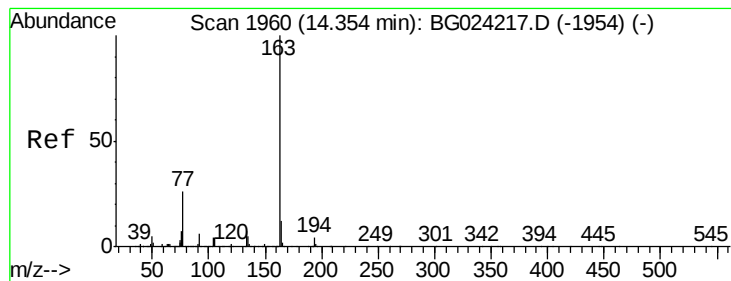

#44

Dimethylphthalate

Concen: 16.77 ng/ul

RT: 14.356 min Scan# 19

Delta R.T. 0.001 min

Lab File: BG024207.D

Acq: 6 Oct 2016 20:15

Instrument :

BNA_G

ClientSampleId :

BDPH2

Tot Ion:163 Resp: 589617

Ion Ratio Lower Upper

163 100

194 4.3 3.4 5.2

164 10.4 8.8 13.2

