

Data Path : Z:\HPCHEM1\BNA G\Data\BG100716\RAW\
 Data File : BG024208.D
 Acq On : 6 Oct 2016 20:54
 Operator : UM/SJ
 Sample : H5082-04
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDPH4

Quant Time: Oct 07 09:26:11 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 07 06:34:32 2016
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.303	152	153839	20.00	ng/ul	0.00
18) Naphthalene-d8	11.129	136	641485	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.912	164	513848	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.750	188	752726	20.00	ng/ul	0.09
75) Chrysene-d12	21.957	240	1164249	20.00	ng/ul	0.00
83) Perylene-d12	25.412	264	1181141	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.655	96	5468	1.69	ng/uL	0.00
5) Phenol-d5	7.427	99	162953	11.35	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	7.615	67	117350	12.09	ng/ul	0.00
9) 2-Chlorophenol-d4	7.827	132	115818	11.72	ng/ul	0.00
13) 4-Methylphenol-d8	8.984	113	109026	9.40	ng/ul	0.00
19) Nitrobenzene-d5	9.472	128	57246	12.57	ng/ul	0.00
22) 2-Nitrophenol-d4	10.206	143	63006	12.37	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.735	165	123332	11.12	ng/ul	0.00
29) 4-Chloroaniline-d4	11.258	131	118403	10.16	ng/ul	0.00
43) Dimethylphthalate-d6	14.313	166	477901	13.32	ng/ul	0.00
46) Acenaphthylene-d8	14.613	160	551644	13.42	ng/ul	0.00
51) 4-Nitrophenol-d4	15.071	143	67911	10.67	ng/ul	0.00
57) Fluorene-d10	15.900	176	485741	14.32	ng/ul	0.00
62) 4,6-Dinitro-2-methylph...	16.105	200	227	0.05	ng/ul	0.11
70) Anthracene-d10	17.809	188	1452	0.04	ng/ul	0.05
76) Pyrene-d10	20.018	212	902168	16.60	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.165	264	822917	15.49	ng/ul	0.00
Target Compounds						
44) Dimethylphthalate	14.354	163	377693	10.74	ng/ul#	Ovalue 97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\Data\BG100716\RAW\
Data File : BG024208.D
Acq On : 6 Oct 2016 20:54
Operator : UM/SJ
Sample : H5082-04
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDPH4

Quant Time: Oct 07 09:26:11 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 07 06:34:32 2016
Response via : Initial Calibration

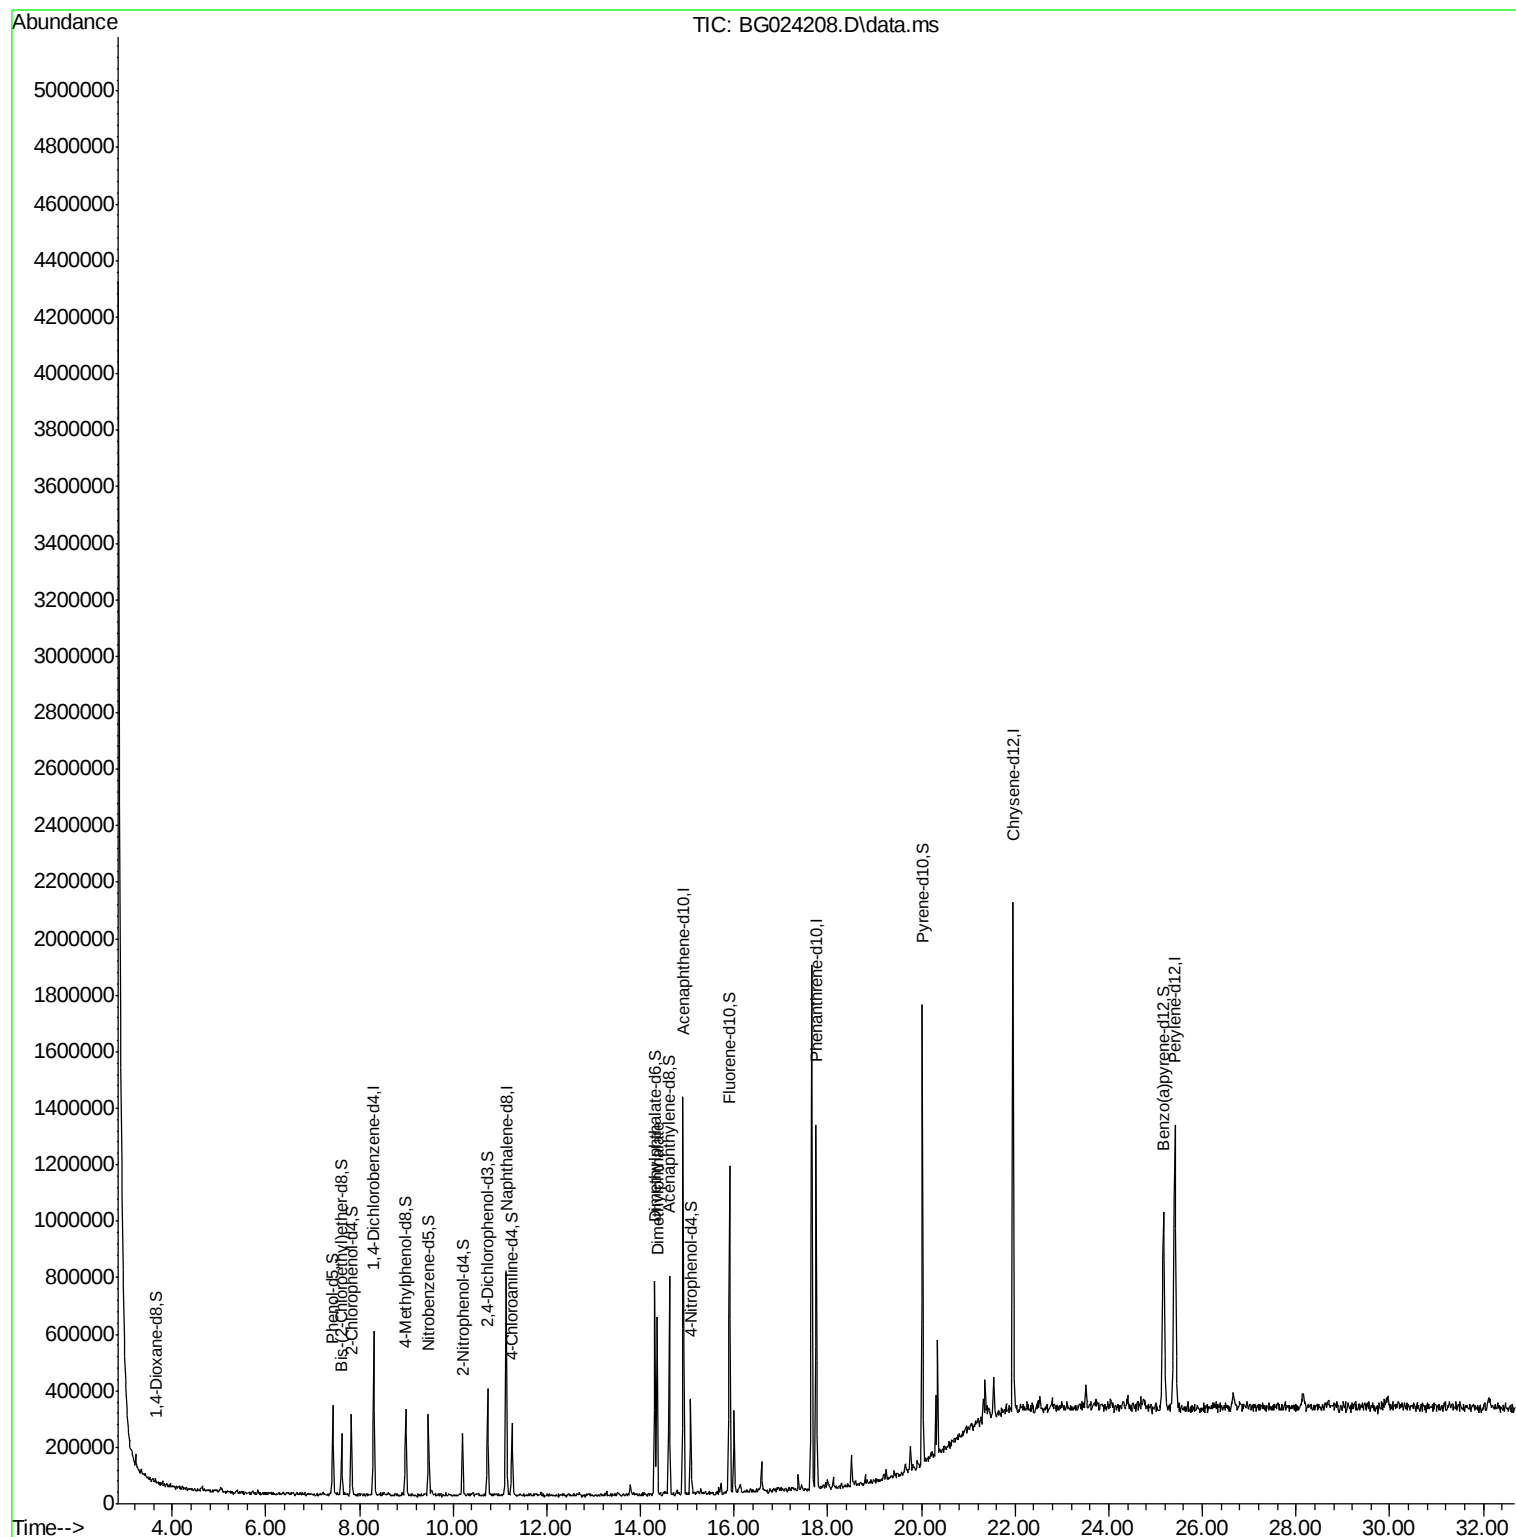

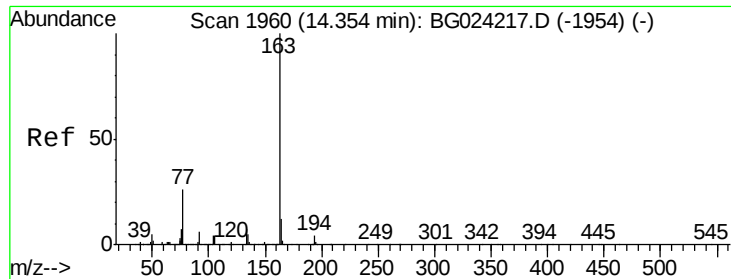

#44

Dimethylphthalate

Concen: 10.74 ng/ul

RT: 14.354 min Scan# 19

Delta R.T. -0.000 min

Lab File: BG024208.D

Acq: 6 Oct 2016 20:54

Instrument :

BNA_G

ClientSampleId :

BDPH4

Tot Ion:163 Resp: 377693

Ion Ratio Lower Upper

163 100

194 5.8 3.4 5.2#

164 11.7 8.8 13.2

