

Data Path : Z:\HPCHEM1\BNA G\Data\BG100716\RAW\
 Data File : BG024209.D
 Acq On : 6 Oct 2016 21:33
 Operator : UM/SJ
 Sample : H5082-05
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDPH8

Quant Time: Oct 07 09:26:35 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 07 06:34:32 2016
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.302	152	166428	20.00	ng/ul	0.00
18) Naphthalene-d8	11.128	136	689412	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.918	164	548198	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.755	188	1795616	20.00	ng/ul	0.10
75) Chrysene-d12	21.951	240	1273948	20.00	ng/ul	0.00
83) Perylene-d12	25.411	264	1277502	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.654	96	17780	5.07	ng/uL	0.00
5) Phenol-d5	7.426	99	441337	28.42	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	7.614	67	308921	29.43	ng/ul	0.00
9) 2-Chlorophenol-d4	7.826	132	317215	29.67	ng/ul	0.00
13) 4-Methylphenol-d8	8.983	113	370069	29.48	ng/ul	0.00
19) Nitrobenzene-d5	9.683	128	186	0.04	ng/ul	0.20
22) 2-Nitrophenol-d4	10.200	143	190397	34.78	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.734	165	355579	29.83	ng/ul	0.00
29) 4-Chloroaniline-d4	11.257	131	476159	38.02	ng/ul	0.00
43) Dimethylphthalate-d6	14.312	166	1265103	33.05	ng/ul	0.00
46) Acenaphthylene-d8	14.612	160	1459536	33.29	ng/ul	0.00
51) 4-Nitrophenol-d4	15.076	143	201454	29.68	ng/ul	0.00
57) Fluorene-d10	15.899	176	1166213	32.23	ng/ul	0.00
62) 4,6-Dinitro-2-methylph...	16.063	200	329	0.03	ng/ul	0.06
70) Anthracene-d10	17.755	188	1795616	22.14	ng/ul	0.00
76) Pyrene-d10	20.023	212	1993209	33.52	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.170	264	2012806	35.02	ng/ul	0.00
Target Compounds						
44) Dimethylphthalate	14.354	163	762303	20.31	ng/ul	Ovalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\Data\BG100716\RAW\
Data File : BG024209.D
Acq On : 6 Oct 2016 21:33
Operator : UM/SJ
Sample : H5082-05
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDPH8

Quant Time: Oct 07 09:26:35 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 07 06:34:32 2016
Response via : Initial Calibration

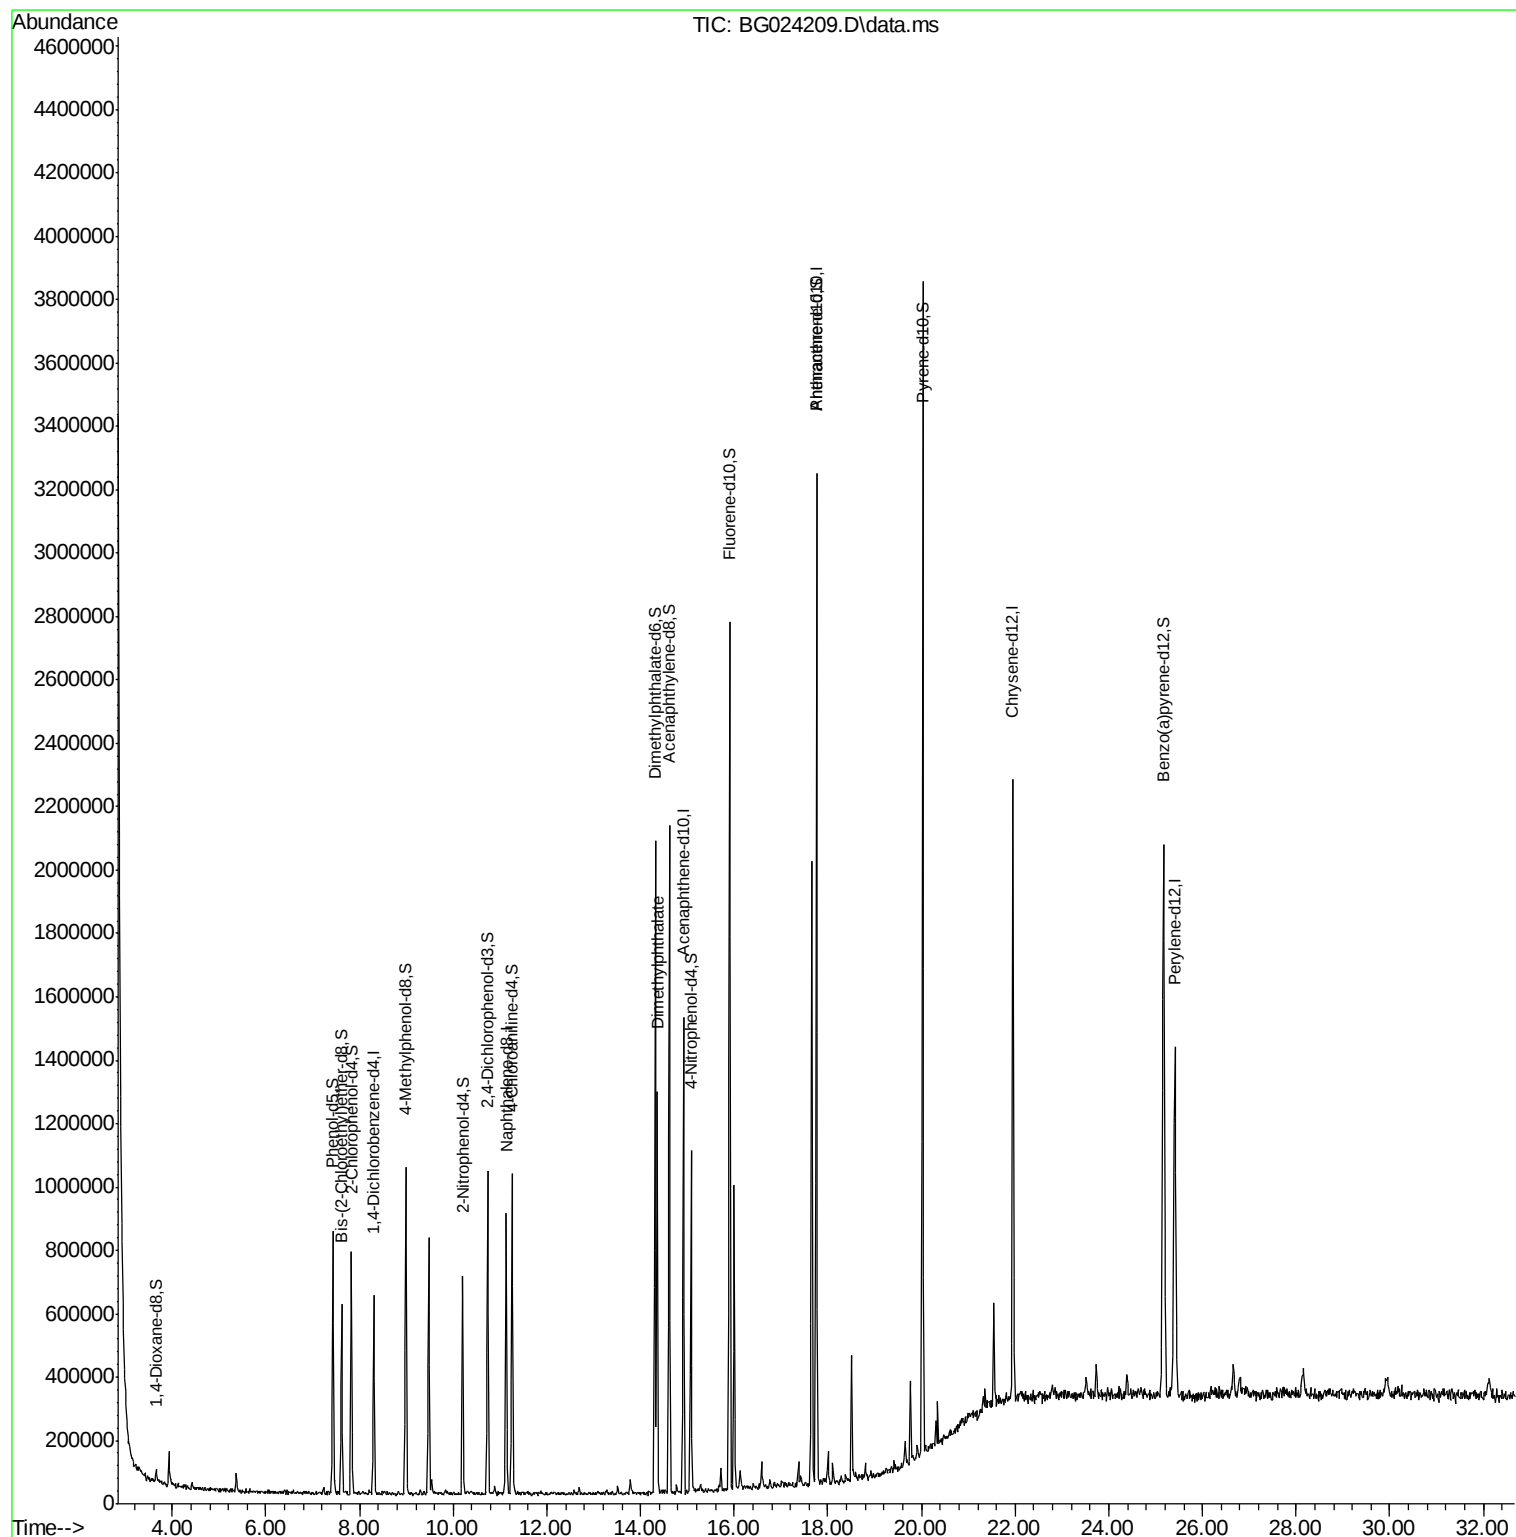

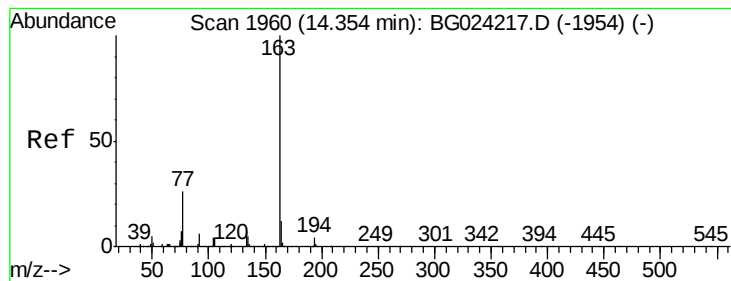

#44

Dimethylphthalate

Concen: 20.31 ng/ul

RT: 14.354 min Scan# 19

Delta R.T. -0.001 min

Lab File: BG024209.D

Acq: 6 Oct 2016 21:33

Instrument :

BNA_G

ClientSampleId :

BDPH8

Tot Ion:163 Resp: 762303

Ion Ratio Lower Upper

163 100

194 4.4 3.4 5.2

164 10.9 8.8 13.2

