

Data Path : Z:\HPCHEM1\BNA G\Data\BG100716\RAW\
 Data File : BG024212.D
 Acq On : 6 Oct 2016 23:29
 Operator : UM/SJ
 Sample : H5082-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDPH5

Quant Time: Oct 07 09:27:51 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 07 06:34:32 2016
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.302	152	158382	20.00	ng/ul	0.00
18) Naphthalene-d8	11.134	136	698260	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.912	164	576878	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.749	188	1805076	20.00	ng/ul	0.09
75) Chrysene-d12	21.950	240	1300123	20.00	ng/ul	0.00
83) Perylene-d12	25.411	264	1303618	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.654	96	17888	5.36	ng/uL	0.00
5) Phenol-d5	7.426	99	453295	30.68	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	7.614	67	327326	32.77	ng/ul	0.00
9) 2-Chlorophenol-d4	7.826	132	321226	31.57	ng/ul	0.00
13) 4-Methylphenol-d8	8.983	113	355008	29.72	ng/ul	0.00
19) Nitrobenzene-d5	9.477	128	169596	34.22	ng/ul	0.00
22) 2-Nitrophenol-d4	10.199	143	193939	34.98	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.734	165	359532	29.78	ng/ul	0.00
29) 4-Chloroaniline-d4	11.257	131	481503	37.95	ng/ul	0.00
43) Dimethylphthalate-d6	14.312	166	1280661	31.79	ng/ul	0.00
46) Acenaphthylene-d8	14.612	160	1463238	31.71	ng/ul	0.00
51) 4-Nitrophenol-d4	15.076	143	210693	29.50	ng/ul	0.00
57) Fluorene-d10	15.899	176	1193659	31.34	ng/ul	0.00
62) 4,6-Dinitro-2-methylph...	16.093	200	258	0.02	ng/ul	0.09
70) Anthracene-d10	17.749	188	1805076	22.14	ng/ul	0.00
76) Pyrene-d10	20.023	212	2040025	33.62	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.170	264	2006238	34.21	ng/ul	0.00
Target Compounds						
44) Dimethylphthalate	14.359	163	699251	17.70	ng/ul	Ovalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\Data\BG100716\RAW\
Data File : BG024212.D
Acq On : 6 Oct 2016 23:29
Operator : UM/SJ
Sample : H5082-11
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDPH5

Quant Time: Oct 07 09:27:51 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 07 06:34:32 2016
Response via : Initial Calibration

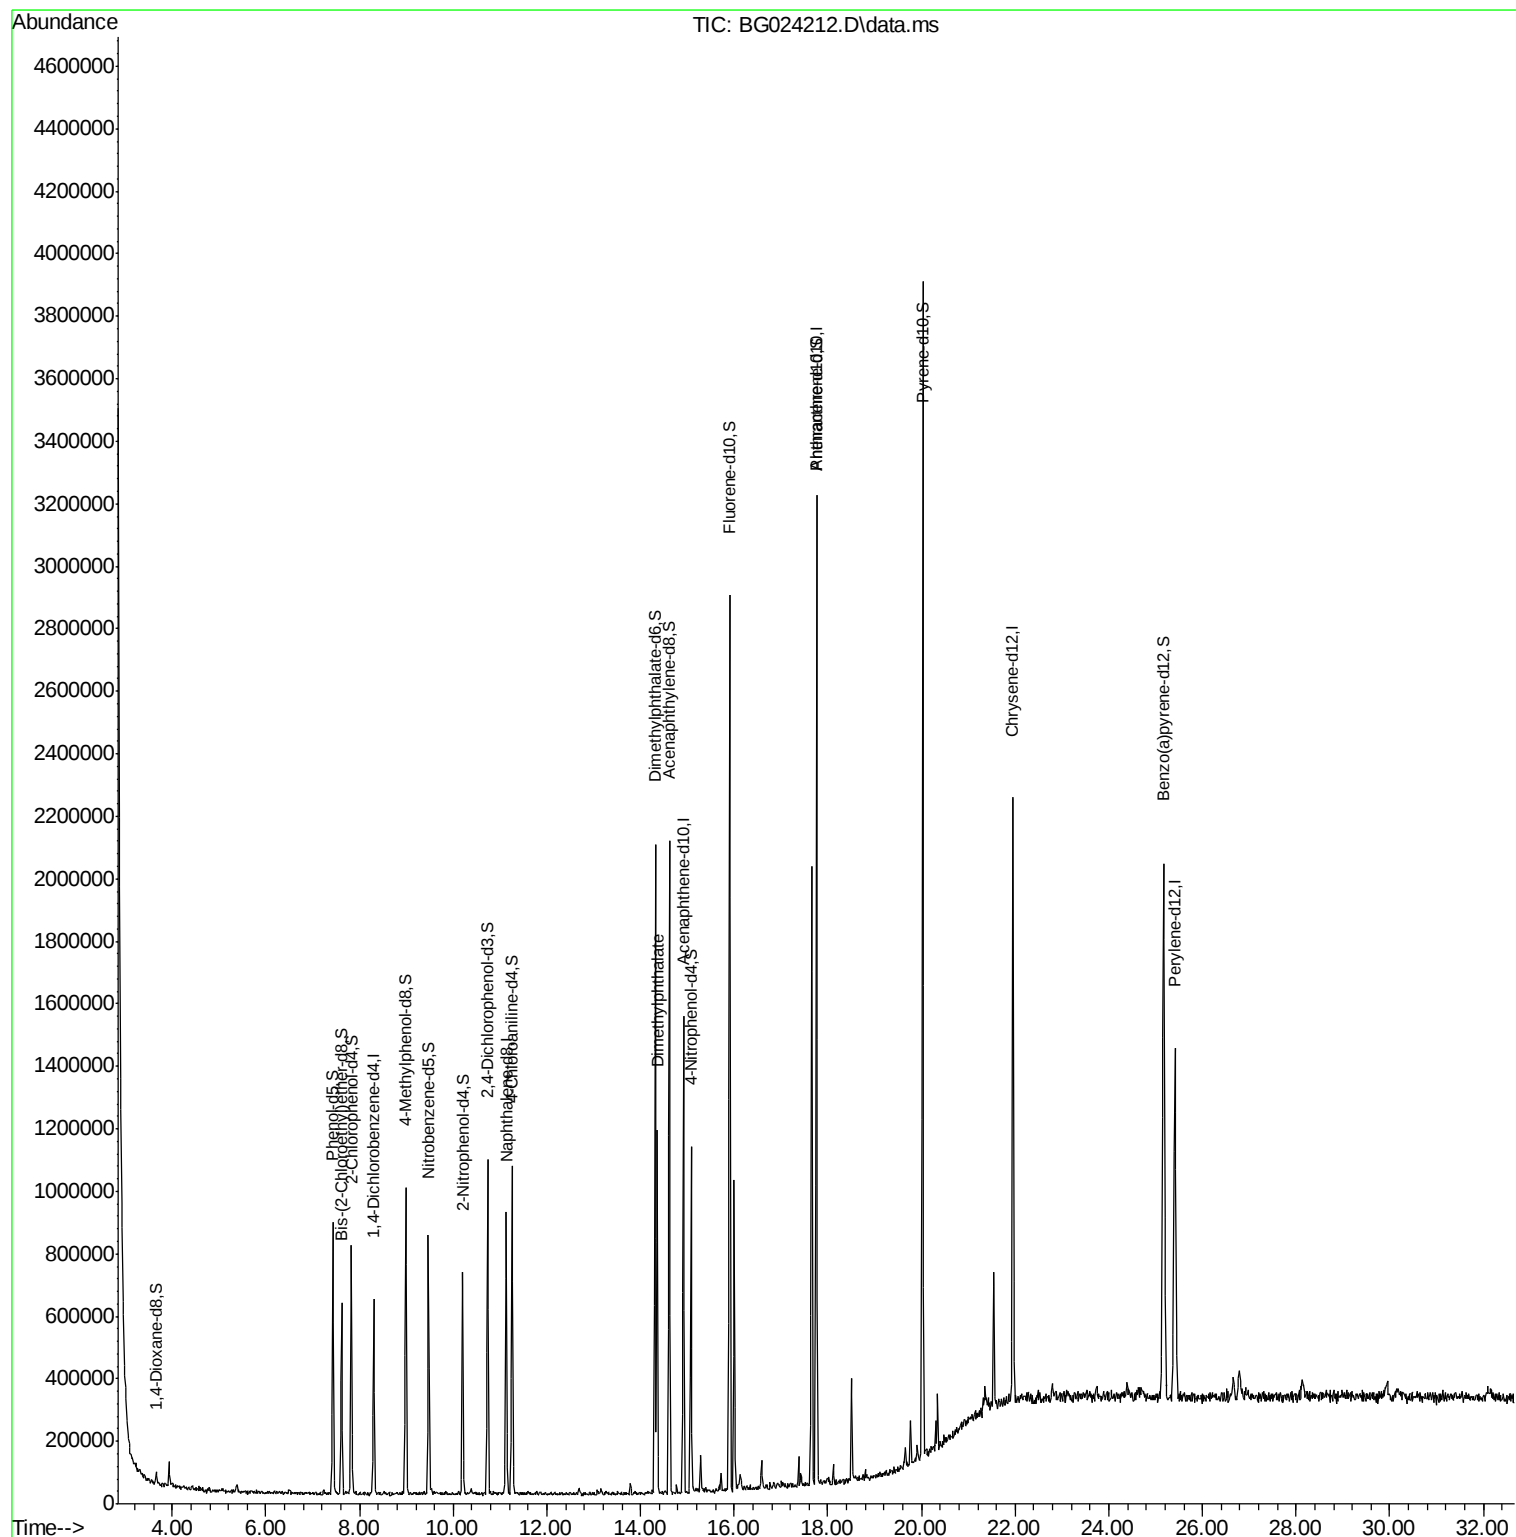

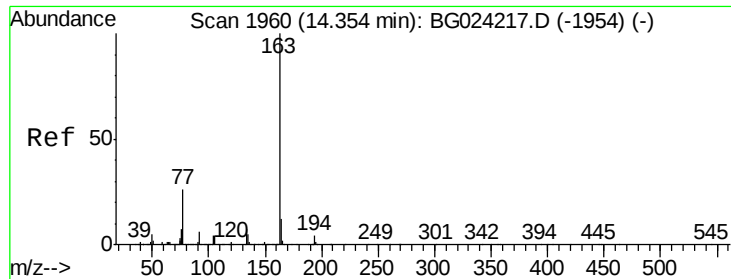

#44

Dimethylphthalate

Concen: 17.70 ng/ul

RT: 14.359 min Scan# 19

Delta R.T. 0.005 min

Lab File: BG024212.D

Acq: 6 Oct 2016 23:29

Instrument :

BNA_G

ClientSampleId :

BDPH5

Tot Ion:163 Resp: 699251

Ion Ratio Lower Upper

163 100

194 4.7 3.4 5.2

164 10.2 8.8 13.2

