

Data Path : Z:\HPCHEM1\BNA G\Data\BG100716\RAW\
 Data File : BG024219.D
 Acq On : 7 Oct 2016 4:08
 Operator : UM/SJ
 Sample : H5082-17
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDPJ6

Quant Time: Oct 07 09:31:31 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 07 06:34:32 2016
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.301	152	146458	20.00	ng/ul	0.00
18) Naphthalene-d8	11.128	136	600064	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.911	164	499798	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.655	188	1082003	20.00	ng/ul	0.00
75) Chrysene-d12	21.950	240	1162274	20.00	ng/ul	0.00
83) Perylene-d12	25.405	264	1150040	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.654	96	12860	4.17	ng/uL	0.00
5) Phenol-d5	7.426	99	346352	25.35	ng/ul	0.00
7) Bis-(2-Chloroethyl)eth...	7.614	67	235364	25.48	ng/ul	0.00
9) 2-Chlorophenol-d4	7.820	132	247176	26.27	ng/ul	0.00
13) 4-Methylphenol-d8	8.983	113	294898	26.70	ng/ul	0.00
19) Nitrobenzene-d5	9.471	128	130132	30.56	ng/ul	0.00
22) 2-Nitrophenol-d4	10.199	143	141882	29.78	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.728	165	274756	26.48	ng/ul	0.00
29) 4-Chloroaniline-d4	11.257	131	316234	29.01	ng/ul	0.00
43) Dimethylphthalate-d6	14.312	166	991939	28.42	ng/ul	0.00
46) Acenaphthylene-d8	14.612	160	1161512	29.06	ng/ul	0.00
51) 4-Nitrophenol-d4	15.076	143	163084	26.36	ng/ul	0.00
57) Fluorene-d10	15.898	176	965787	29.27	ng/ul	0.00
62) 4,6-Dinitro-2-methylph...	15.998	200	158180	24.33	ng/ul	0.00
70) Anthracene-d10	17.755	188	1480175	30.29	ng/ul	0.00
76) Pyrene-d10	20.017	212	1647838	30.38	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.170	264	1605031	31.02	ng/ul	0.00
Target Compounds						
44) Dimethylphthalate	14.353	163	807663	23.60	ng/ul	Ovalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\Data\BG100716\RAW\
Data File : BG024219.D
Acq On : 7 Oct 2016 4:08
Operator : UM/SJ
Sample : H5082-17
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDPJ6

Quant Time: Oct 07 09:31:31 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 07 06:34:32 2016
Response via : Initial Calibration

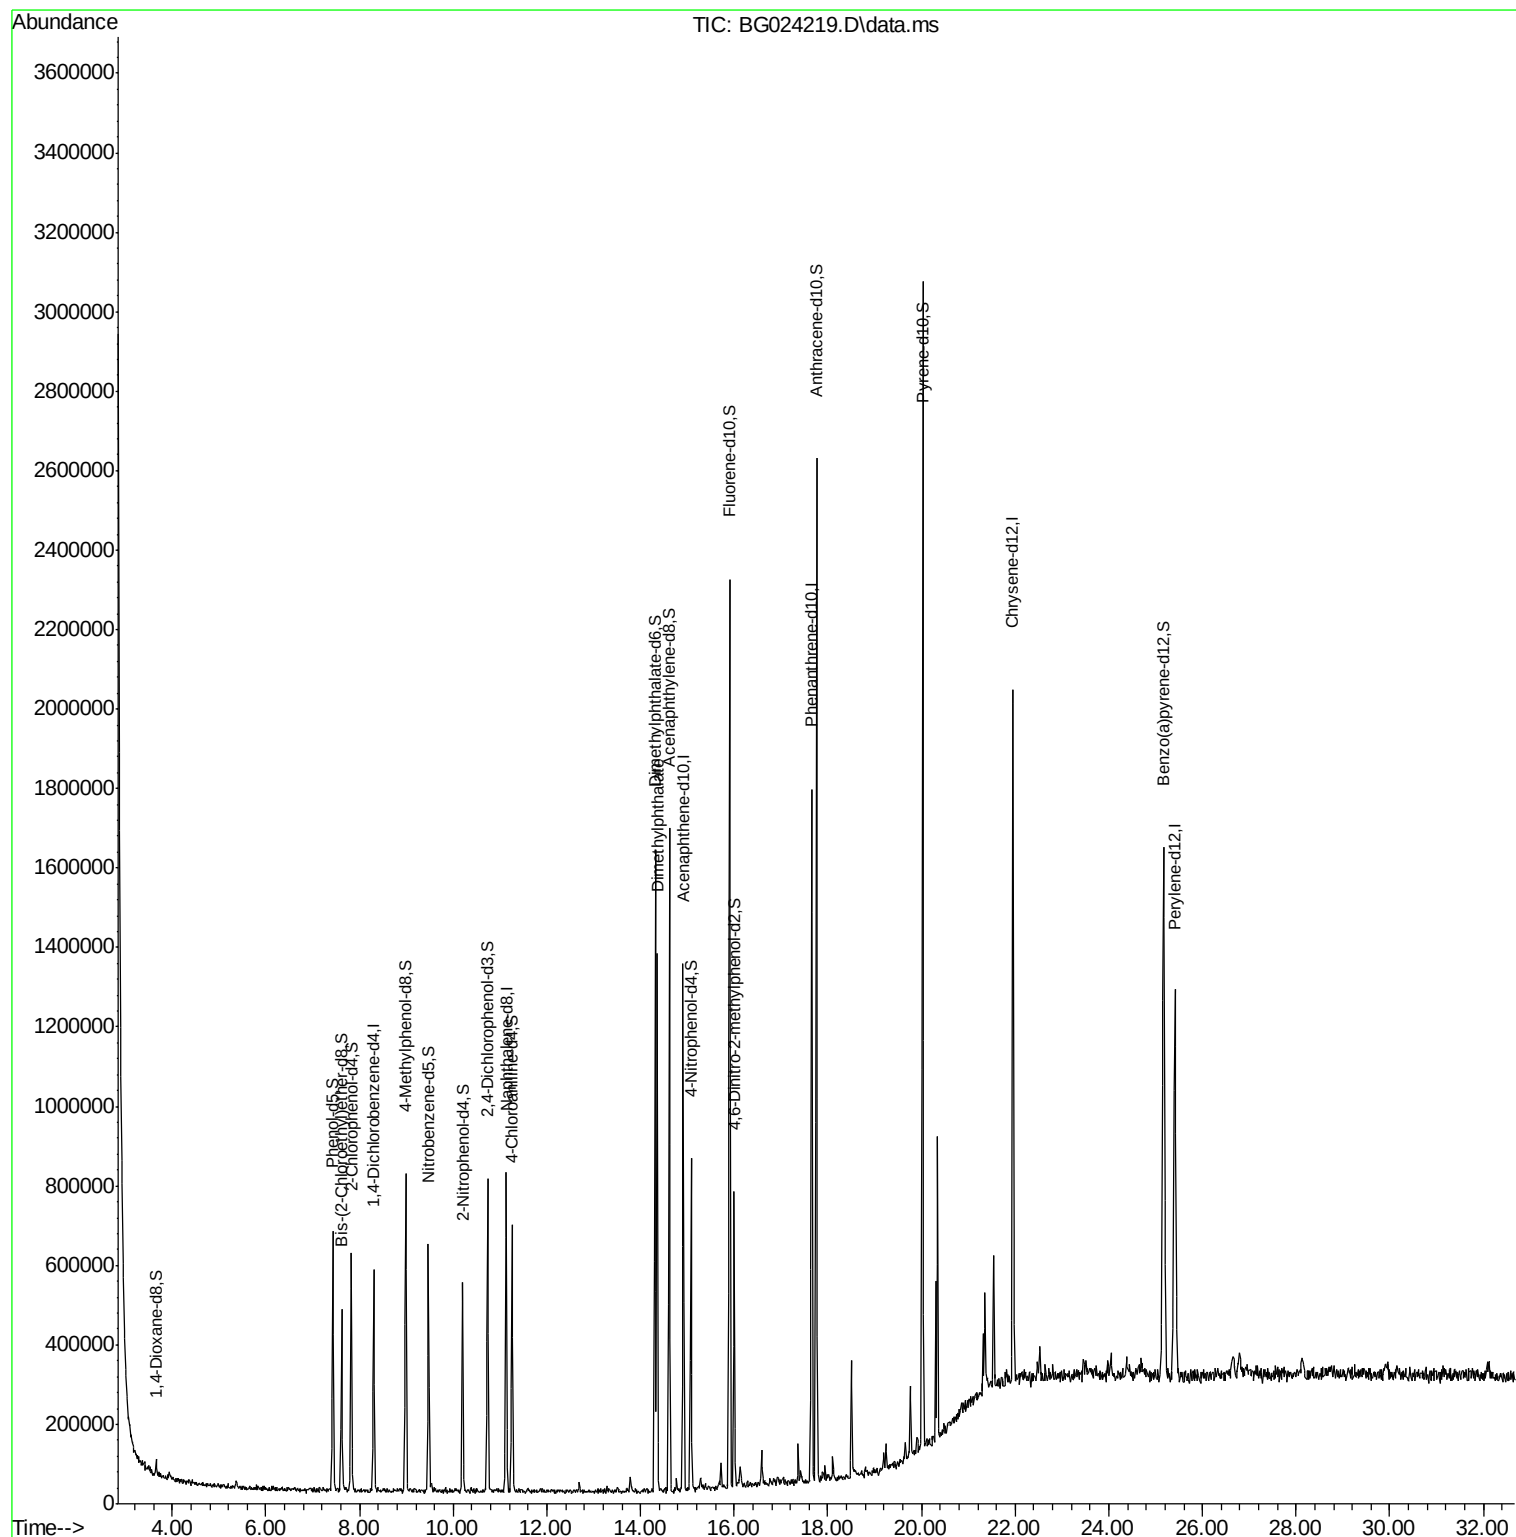

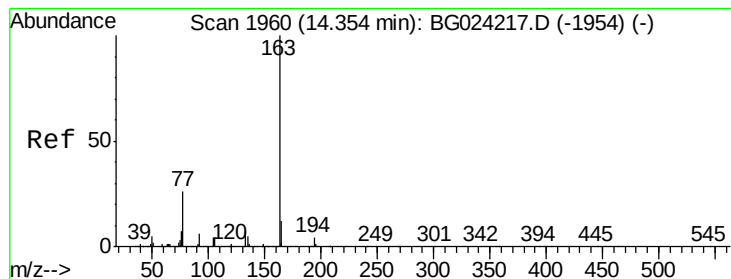

#44

Dimethylphthalate

Concen: 23.60 ng/ul

RT: 14.353 min Scan# 19

Delta R.T. -0.001 min

Lab File: BG024219.D

Acq: 7 Oct 2016 4:08

Instrument :

BNA_G

ClientSampleId :

BDPJ6

Tot Ion:163 Resp: 807663

Ion Ratio Lower Upper

163 100

194 4.0 3.4 5.2

164 11.7 8.8 13.2

