

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG100716\
 Data File : BG024212.D
 Acq On : 6 Oct 2016 23:29
 Operator : UM/SJ
 Sample : H5082-11
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDPH5

Manual Integrations
 APPROVED

sohil
 10/7/2016 6:59:45 PM

Quant Time: Oct 07 01:34:57 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG0100716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 07 00:50:12 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.30	152	158382	20.00	ng/ul	0.00
18) Naphthalene-d8	11.13	136	698260	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.91	164	576878	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.66	188	1193800m	20.00	ng/ul	0.00
75) Chrysene-d12	21.95	240	1300123	20.00	ng/ul	0.00
83) Perylene-d12	25.41	264	1303618	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.65	96	17888	5.36	ng/uL	0.00
5) Phenol-d5	7.43	99	453295	30.68	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.61	67	327326	32.77	ng/ul	0.00
9) 2-Chlorophenol-d4	7.83	132	321226	31.57	ng/ul	0.00
13) 4-Methylphenol-d8	8.98	113	355008	29.72	ng/ul	0.00
19) Nitrobenzene-d5	9.48	128	169596	34.22	ng/ul	0.00
22) 2-Nitrophenol-d4	10.20	143	193939	34.98	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.73	165	359532	29.78	ng/ul	0.00
29) 4-Chloroaniline-d4	11.26	131	481503	37.95	ng/ul	0.00
43) Dimethylphthalate-d6	14.31	166	1280661	31.79	ng/ul	0.00
46) Acenaphthylene-d8	14.61	160	1463238	31.71	ng/ul	0.00
51) 4-Nitrophenol-d4	15.08	143	210693	29.50	ng/ul	0.00
57) Fluorene-d10	15.90	176	1193659	31.34	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.00	200	219626m	30.61	ng/ul	0.00
70) Anthracene-d10	17.75	188	1805076	33.47	ng/ul	0.00
76) Pyrene-d10	20.02	212	2040025	33.62	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.17	264	2006238	34.21	ng/ul	0.00

Target Compounds					Qvalue
44) Dimethylphthalate	14.36	163	699251	17.70 ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG100716\
Data File : BG024212.D
Acq On : 6 Oct 2016 23:29
Operator : UM/SJ
Sample : H5082-11
Misc :
ALS Vial : 14 Sample Multiplier: 1




Instrument :
BNA_G
ClientSampleId :
BDPH5

Manual Integrations
APPROVED

sohil
10/7/2016 6:59:45 PM

Quant Time: Oct 07 01:34:57 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG0100716.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 07 00:50:12 2016
Response via : Initial Calibration

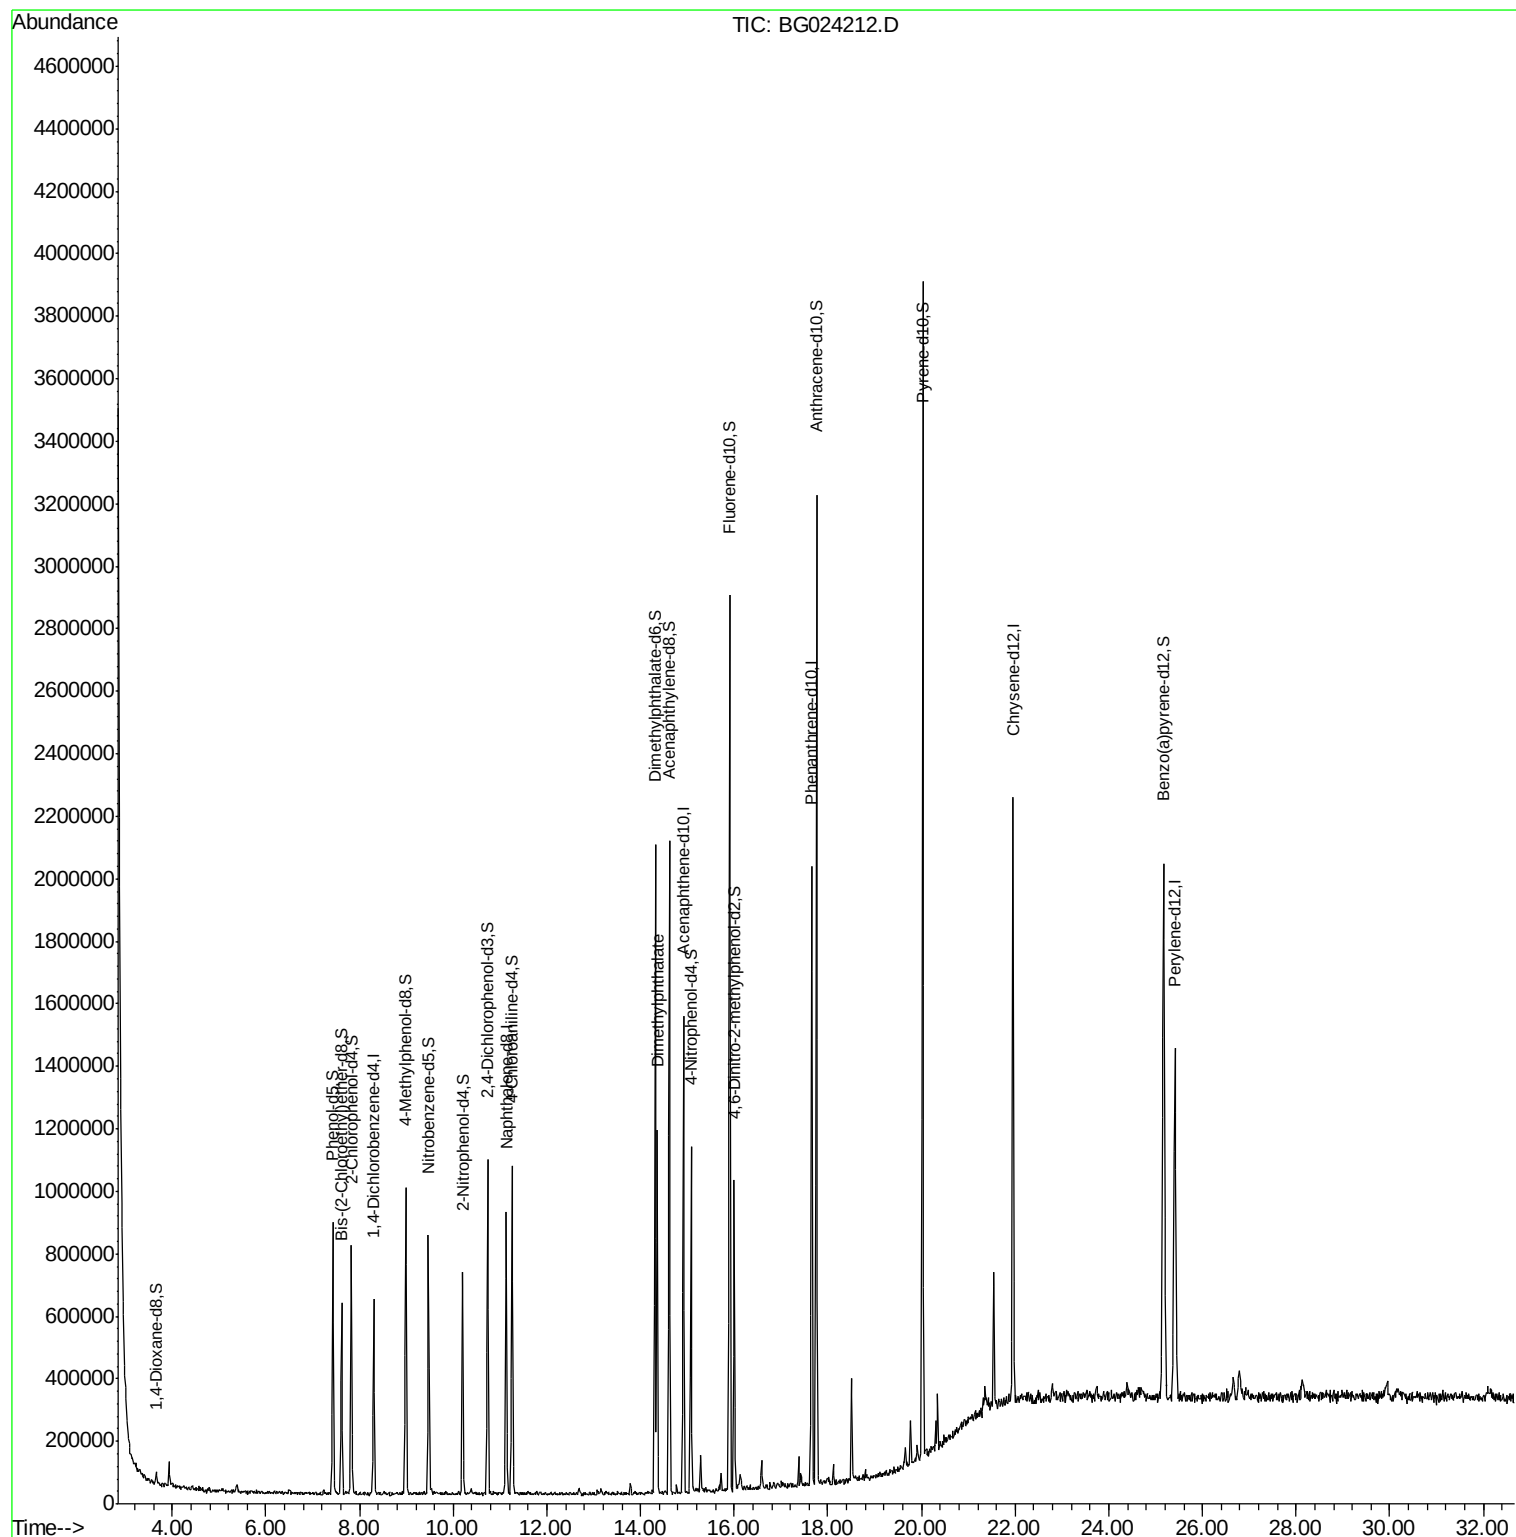

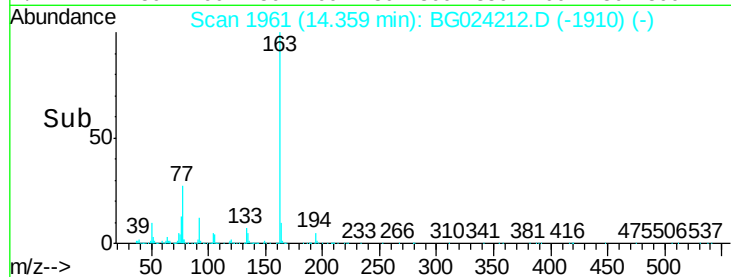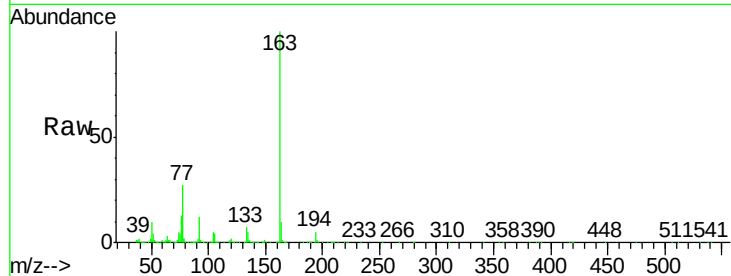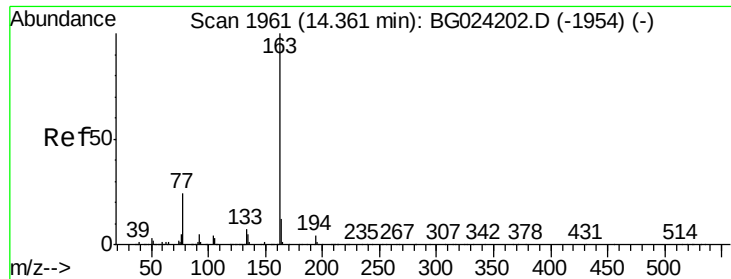

#44

Dimethylphthalate

Concen: 17.70 ng/ul

RT: 14.36 min Scan# 1961

Delta R.T. -0.00 min

Lab File: BG024212.D

Acq: 6 Oct 2016 23:29

Instrument :

BNA_G

ClientSampleId :

BDPH5

Tgt	Ion	Ratio	Resp	Lower	Upper
163	100		699251		
194	4.7	3.4	5.2		
164	10.2	8.8	13.2		

Manual Integrations
APPROVED

sohil
10/7/2016 6:59:45 PM

