

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG100716\
 Data File : BG024213.D
 Acq On : 7 Oct 2016 00:08
 Operator : UM/SJ
 Sample : H5082-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDPH6

Quant Time: Oct 07 00:52:08 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG0100716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 07 00:50:12 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.30	152	157916	20.00	ng/ul	0.00
18) Naphthalene-d8	11.13	136	706920	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.91	164	569315	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.66	188	1218053	20.00	ng/ul	0.00
75) Chrysene-d12	21.95	240	1317065	20.00	ng/ul	0.00
83) Perylene-d12	25.41	264	1310548	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.65	96	13447	4.04	ng/uL	0.00
5) Phenol-d5	7.43	99	391992	26.60	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.61	67	289006	29.02	ng/ul	0.00
9) 2-Chlorophenol-d4	7.82	132	277472	27.35	ng/ul	0.00
13) 4-Methylphenol-d8	8.98	113	335038	28.13	ng/ul	0.00
19) Nitrobenzene-d5	9.47	128	143996	28.70	ng/ul	0.00
22) 2-Nitrophenol-d4	10.20	143	163318	29.10	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.73	165	319348	26.12	ng/ul	0.00
29) 4-Chloroaniline-d4	11.26	131	428433	33.36	ng/ul	0.00
43) Dimethylphthalate-d6	14.31	166	1116621	28.09	ng/ul	0.00
46) Acenaphthylene-d8	14.61	160	1298281	28.51	ng/ul	0.00
51) 4-Nitrophenol-d4	15.08	143	183997	26.10	ng/ul	0.00
57) Fluorene-d10	15.90	176	1035482	27.55	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.00	200	187584	25.63	ng/ul	0.00
70) Anthracene-d10	17.76	188	1554540	28.25	ng/ul	0.00
76) Pyrene-d10	20.02	212	1762878	28.68	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.17	264	1701223	28.85	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	14.35	163	623666	16.00	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG100716\
Data File : BG024213.D
Acq On : 7 Oct 2016 00:08
Operator : UM/SJ
Sample : H5082-12
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDPH6

Quant Time: Oct 07 00:52:08 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG0100716.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 07 00:50:12 2016
Response via : Initial Calibration

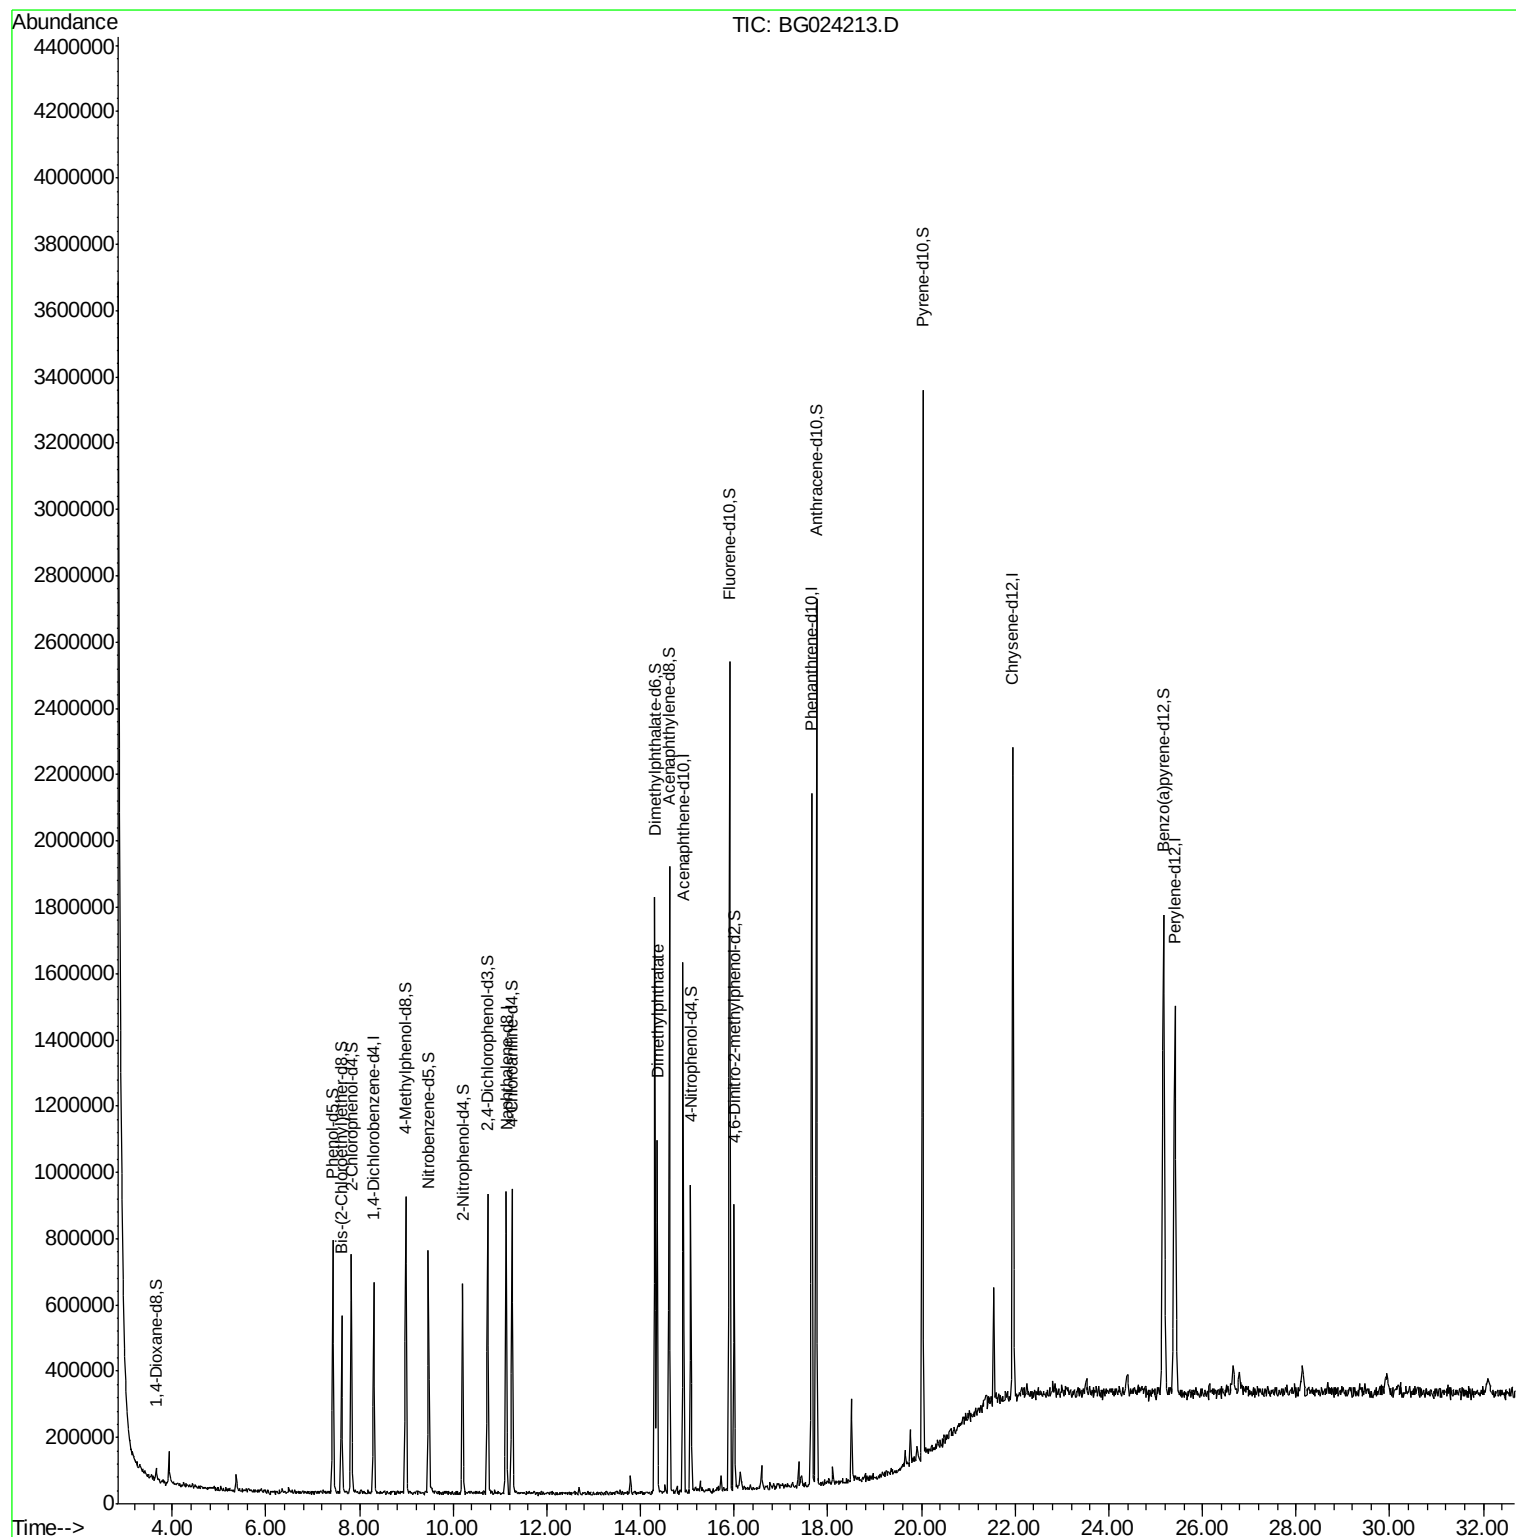

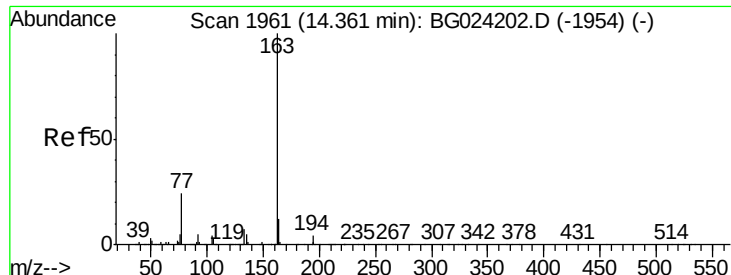

#44

Dimethylphthalate

Concen: 16.00 ng/ul

RT: 14.35 min Scan# 1960

Delta R.T. -0.01 min

Lab File: BG024213.D

Acq: 7 Oct 2016 00:08

Instrument :

BNA_G

ClientSampleId :

BDPH6


Tgt Ion:163 Resp: 623666

Ion Ratio Lower Upper

163 100

194 4.5 3.4 5.2

164 10.4 8.8 13.2

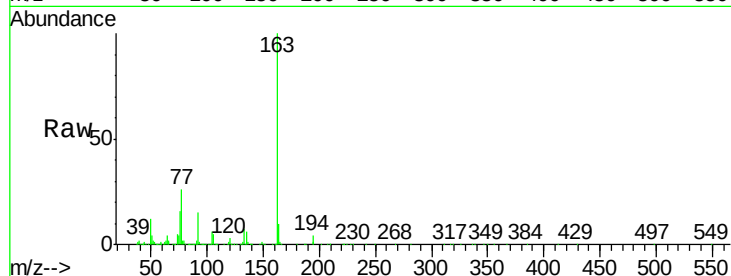

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

