

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG100716\
 Data File : BG024215.D
 Acq On : 7 Oct 2016 1:25
 Operator : UM/SJ
 Sample : H5082-14
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDPJ3

Quant Time: Oct 07 06:16:59 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG0100716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 07 00:50:12 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.30	152	158864	20.00	ng/ul	0.00
18) Naphthalene-d8	11.13	136	688902	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.91	164	544476	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.66	188	1151207	20.00	ng/ul	0.00
75) Chrysene-d12	21.95	240	1232259	20.00	ng/ul	0.00
83) Perylene-d12	25.41	264	1245184	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.65	96	2520	0.75	ng/uL	0.00
5) Phenol-d5	7.43	99	99329	6.70	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.61	67	99480	9.93	ng/ul	0.00
9) 2-Chlorophenol-d4	7.82	132	86853	8.51	ng/ul	0.00
13) 4-Methylphenol-d8	8.98	113	43228	3.61	ng/ul	0.00
19) Nitrobenzene-d5	9.47	128	47713	9.76	ng/ul	0.00
22) 2-Nitrophenol-d4	10.19	143	45962	8.40	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.73	165	88374	7.42	ng/ul	0.00
29) 4-Chloroaniline-d4	11.26	131	27603	2.21	ng/ul	0.00
43) Dimethylphthalate-d6	14.31	166	346257	9.11	ng/ul	0.00
46) Acenaphthylene-d8	14.61	160	435128	9.99	ng/ul	0.00
51) 4-Nitrophenol-d4	15.07	143	30321	4.50	ng/ul	0.00
57) Fluorene-d10	15.90	176	360235	10.02	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.00	200	22839	3.30	ng/ul	0.00
70) Anthracene-d10	17.75	188	535117	10.29	ng/ul	0.00
76) Pyrene-d10	20.02	212	606264	10.54	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.16	264	394994	7.05	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	14.35	163	307439	8.25	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG100716\
Data File : BG024215.D
Acq On : 7 Oct 2016 1:25
Operator : UM/SJ
Sample : H5082-14
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDPJ3

Quant Time: Oct 07 06:16:59 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG0100716.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 07 00:50:12 2016
Response via : Initial Calibration

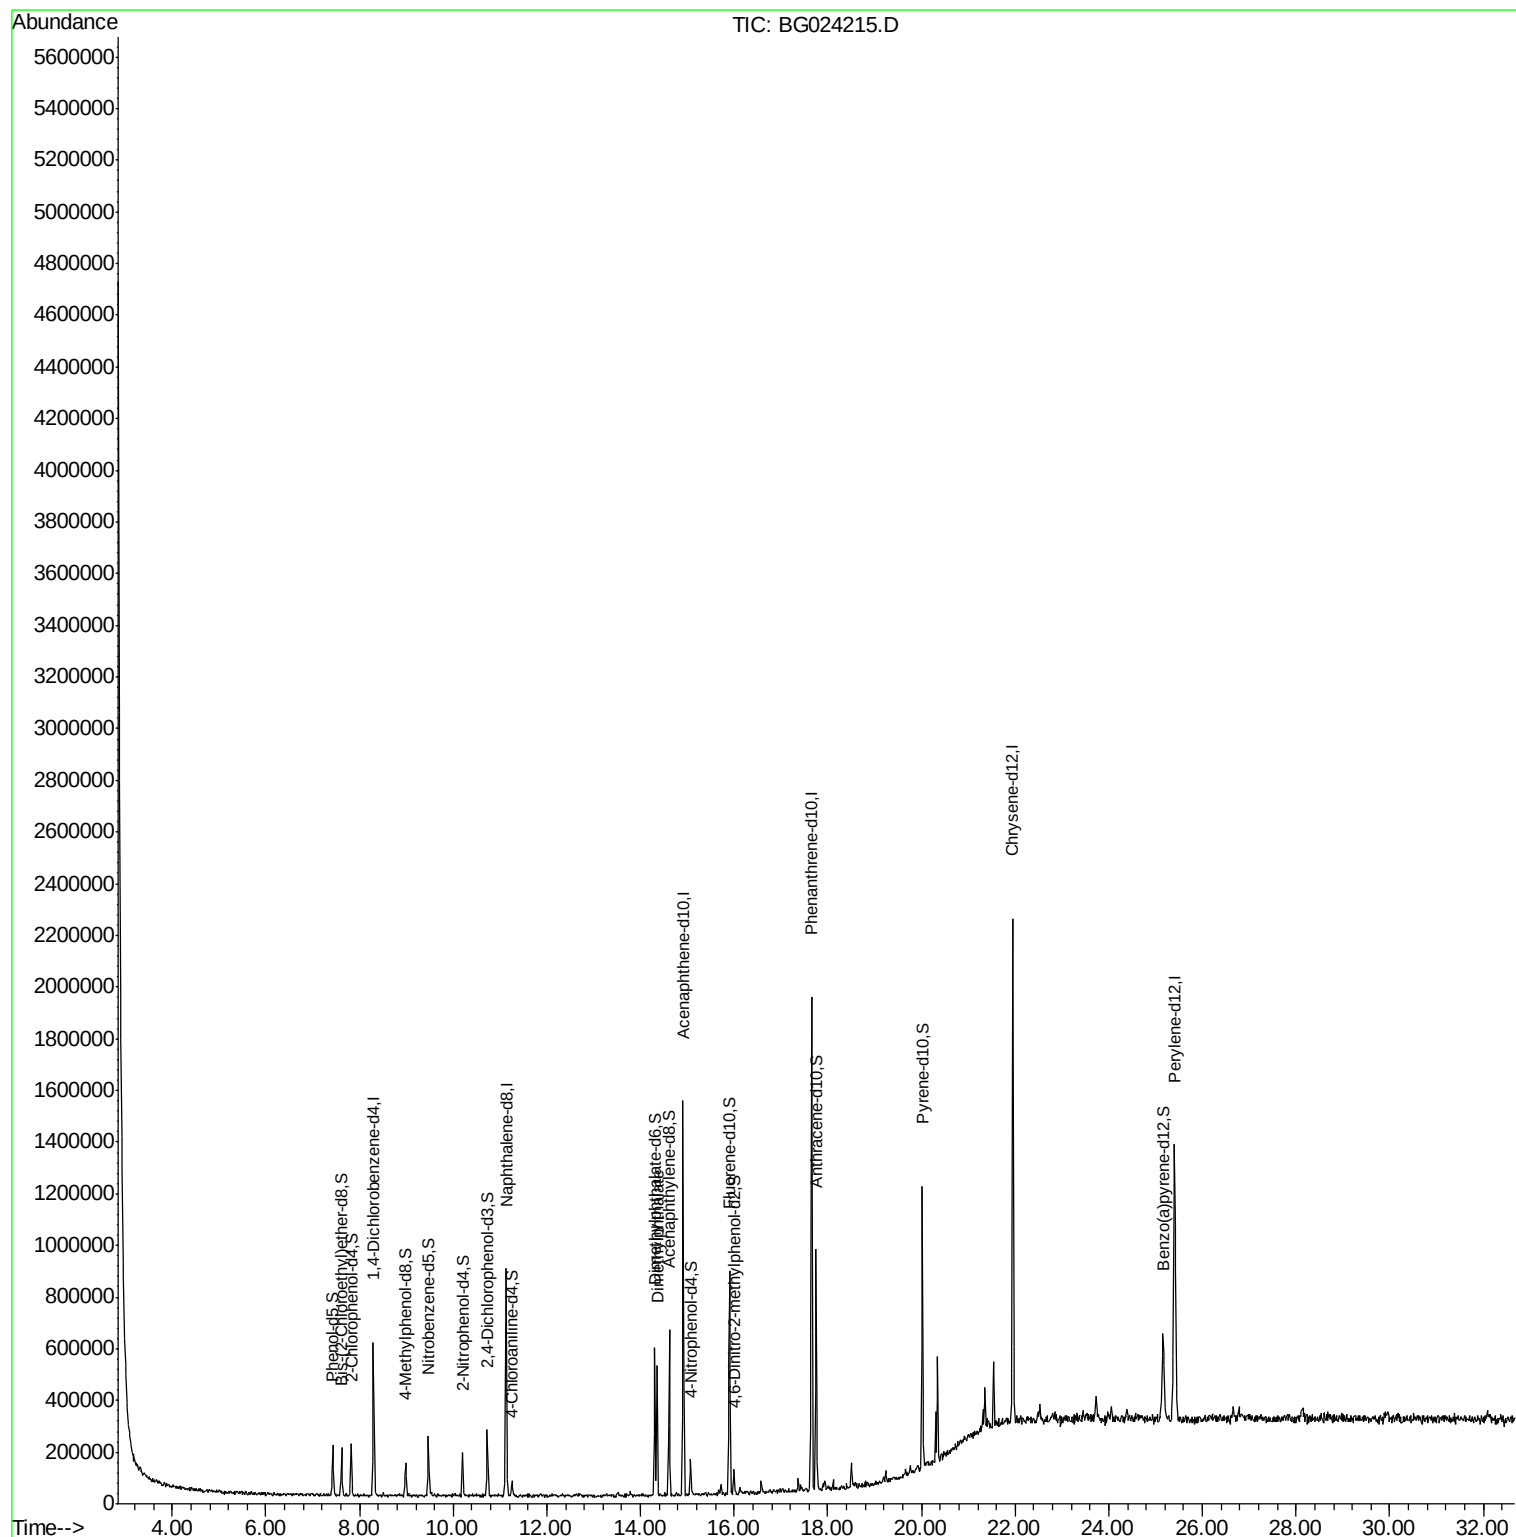

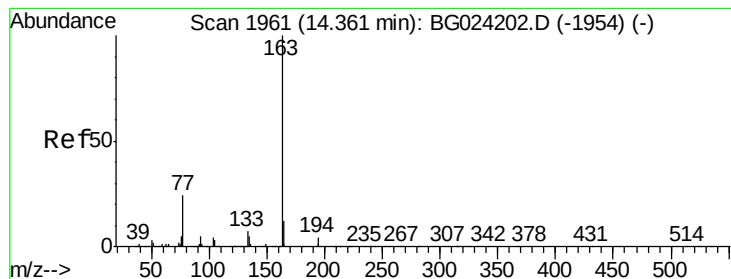

#44

Dimethylphthalate

Concen: 8.25 ng/ul

RT: 14.35 min Scan# 1960

Delta R.T. -0.01 min

Lab File: BG024215.D


Acq: 7 Oct 2016 1:25

Instrument :

BNA_G

ClientSampleId :

BDPJ3

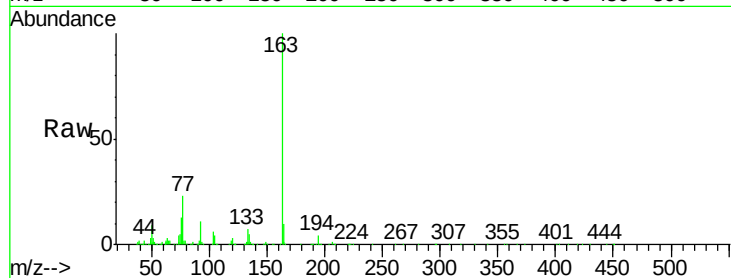

Tgt Ion:	163	Resp:	307439
Ion	Ratio	Lower	Upper
163	100		
194	3.6	3.4	5.2
164	10.3	8.8	13.2

