

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG100716\
 Data File : BG024218.D
 Acq On : 7 Oct 2016 3:29
 Operator : UM/SJ
 Sample : H5082-16
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDPJ5

Quant Time: Oct 07 06:35:27 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG0100716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 07 06:34:32 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.30	152	154522	20.00	ng/ul	0.00
18) Naphthalene-d8	11.13	136	686797	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.92	164	555644	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.65	188	1177349	20.00	ng/ul	0.00
75) Chrysene-d12	21.96	240	1257171	20.00	ng/ul	0.00
83) Perylene-d12	25.41	264	1217395	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.65	96	8163	2.51	ng/uL	0.00
5) Phenol-d5	7.43	99	355993	24.69	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.61	67	260923	26.77	ng/ul	0.00
9) 2-Chlorophenol-d4	7.82	132	253180	25.50	ng/ul	0.00
13) 4-Methylphenol-d8	8.99	113	289637	24.85	ng/ul	0.00
19) Nitrobenzene-d5	9.48	128	138201	28.35	ng/ul	0.00
22) 2-Nitrophenol-d4	10.20	143	149164	27.35	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.73	165	297141	25.02	ng/ul	0.00
29) 4-Chloroaniline-d4	11.26	131	178222	14.28	ng/ul	0.00
43) Dimethylphthalate-d6	14.31	166	890327	22.95	ng/ul	0.00
46) Acenaphthylene-d8	14.62	160	1224402	27.55	ng/ul	0.00
51) 4-Nitrophenol-d4	15.08	143	122604	17.82	ng/ul	0.00
57) Fluorene-d10	15.90	176	991155	27.02	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.00	200	121393	17.16	ng/ul	0.00
70) Anthracene-d10	17.75	188	1465631	27.56	ng/ul	0.00
76) Pyrene-d10	20.02	212	1651667	28.15	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.18	264	1523665	27.82	ng/ul	0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
44) Dimethylphthalate	14.36	163	723855	19.03	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG100716\
Data File : BG024218.D
Acq On : 7 Oct 2016 3:29
Operator : UM/SJ
Sample : H5082-16
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDPJ5

Quant Time: Oct 07 06:35:27 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG0100716.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 07 06:34:32 2016
Response via : Initial Calibration

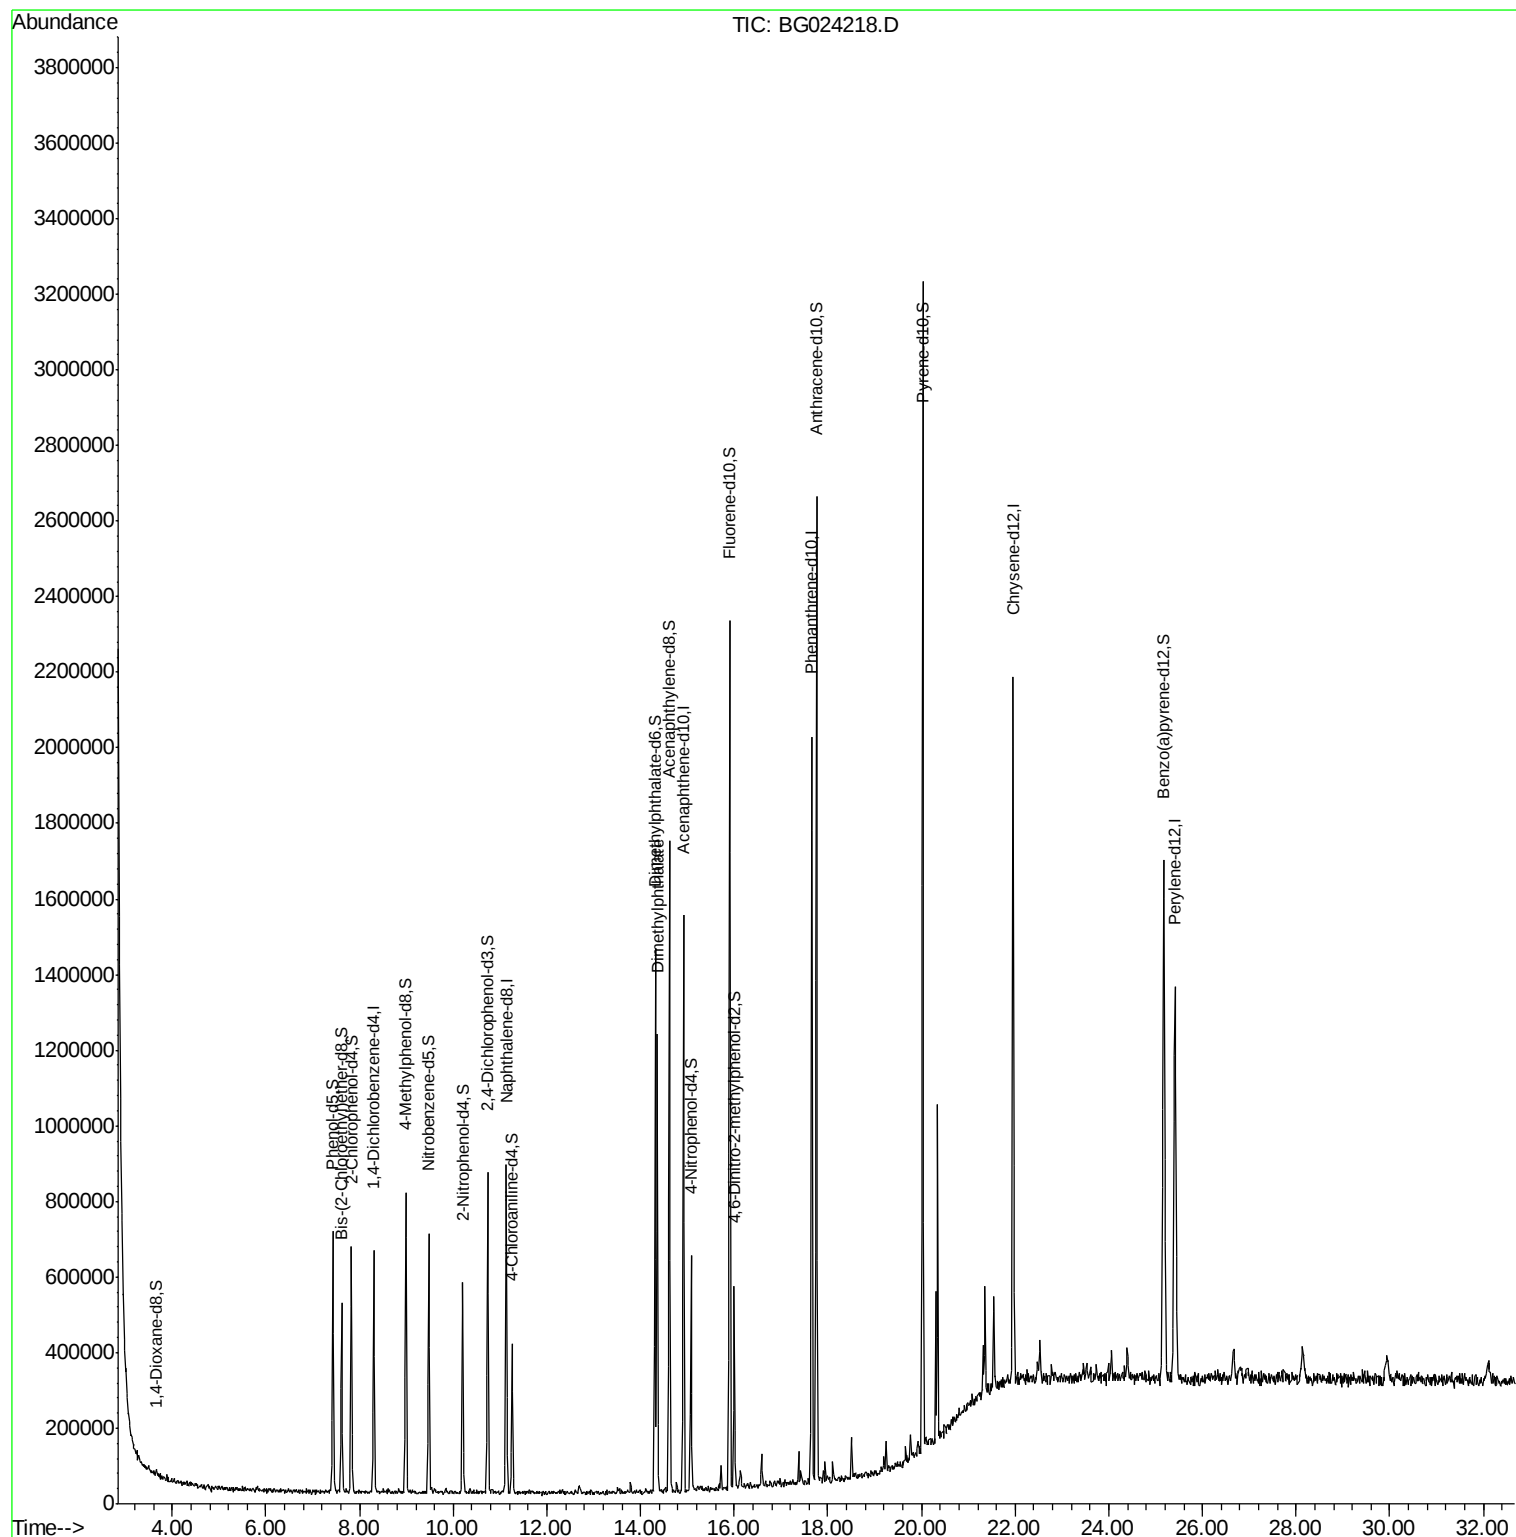

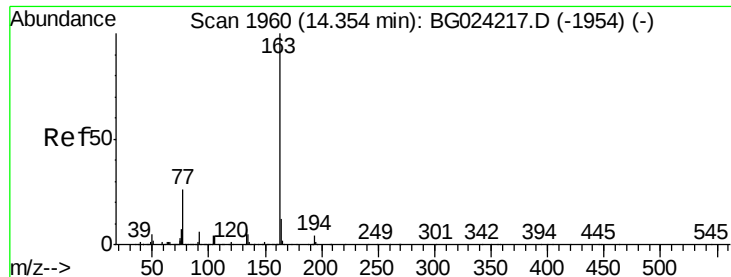

#44

Dimethylphthalate

Concen: 19.03 ng/ul

RT: 14.36 min Scan# 1961

Delta R.T. 0.00 min

Lab File: BG024218.D

Acq: 7 Oct 2016 3:29

Instrument :

BNA_G

ClientSampleId :

BDPJ5


Tgt Ion:163 Resp: 723855

Ion Ratio Lower Upper

163 100

194 5.0 3.4 5.2

164 10.9 8.8 13.2

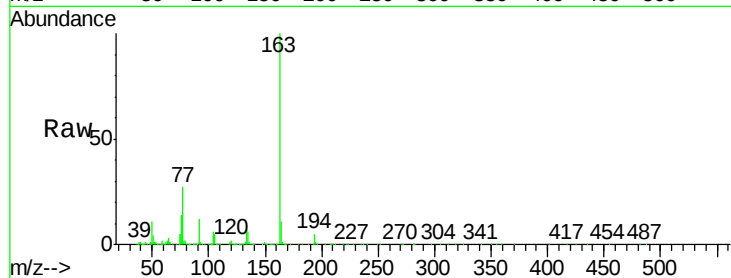

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

