

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG100716\
 Data File : BG024219.D
 Acq On : 7 Oct 2016 4:08
 Operator : UM/SJ
 Sample : H5082-17
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDPJ6

Quant Time: Oct 07 06:35:36 2016
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG0100716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 07 06:34:32 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.30	152	146458	20.00	ng/ul	0.00
18) Naphthalene-d8	11.13	136	600064	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.91	164	499798	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.66	188	1082003	20.00	ng/ul	0.00
75) Chrysene-d12	21.95	240	1162274	20.00	ng/ul	0.00
83) Perylene-d12	25.40	264	1150040	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.65	96	12860	4.17	ng/uL	0.00
5) Phenol-d5	7.43	99	346352	25.35	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.61	67	235364	25.48	ng/ul	0.00
9) 2-Chlorophenol-d4	7.82	132	247176	26.27	ng/ul	0.00
13) 4-Methylphenol-d8	8.98	113	294898	26.70	ng/ul	0.00
19) Nitrobenzene-d5	9.47	128	130132	30.56	ng/ul	0.00
22) 2-Nitrophenol-d4	10.20	143	141882	29.78	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.73	165	274756	26.48	ng/ul	0.00
29) 4-Chloroaniline-d4	11.26	131	316234	29.01	ng/ul	0.00
43) Dimethylphthalate-d6	14.31	166	991939	28.42	ng/ul	0.00
46) Acenaphthylene-d8	14.61	160	1161512	29.06	ng/ul	0.00
51) 4-Nitrophenol-d4	15.08	143	163084	26.36	ng/ul	0.00
57) Fluorene-d10	15.90	176	965787	29.27	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.00	200	158180	24.33	ng/ul	0.00
70) Anthracene-d10	17.76	188	1480175	30.29	ng/ul	0.00
76) Pyrene-d10	20.02	212	1647838	30.38	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.17	264	1605031	31.02	ng/ul	0.00


Target Compounds						Qvalue
44) Dimethylphthalate	14.35	163	807663	23.60	ng/ul	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG100716\
Data File : BG024219.D
Acq On : 7 Oct 2016 4:08
Operator : UM/SJ
Sample : H5082-17
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDPJ6

Quant Time: Oct 07 06:35:36 2016
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG0100716.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 07 06:34:32 2016
Response via : Initial Calibration

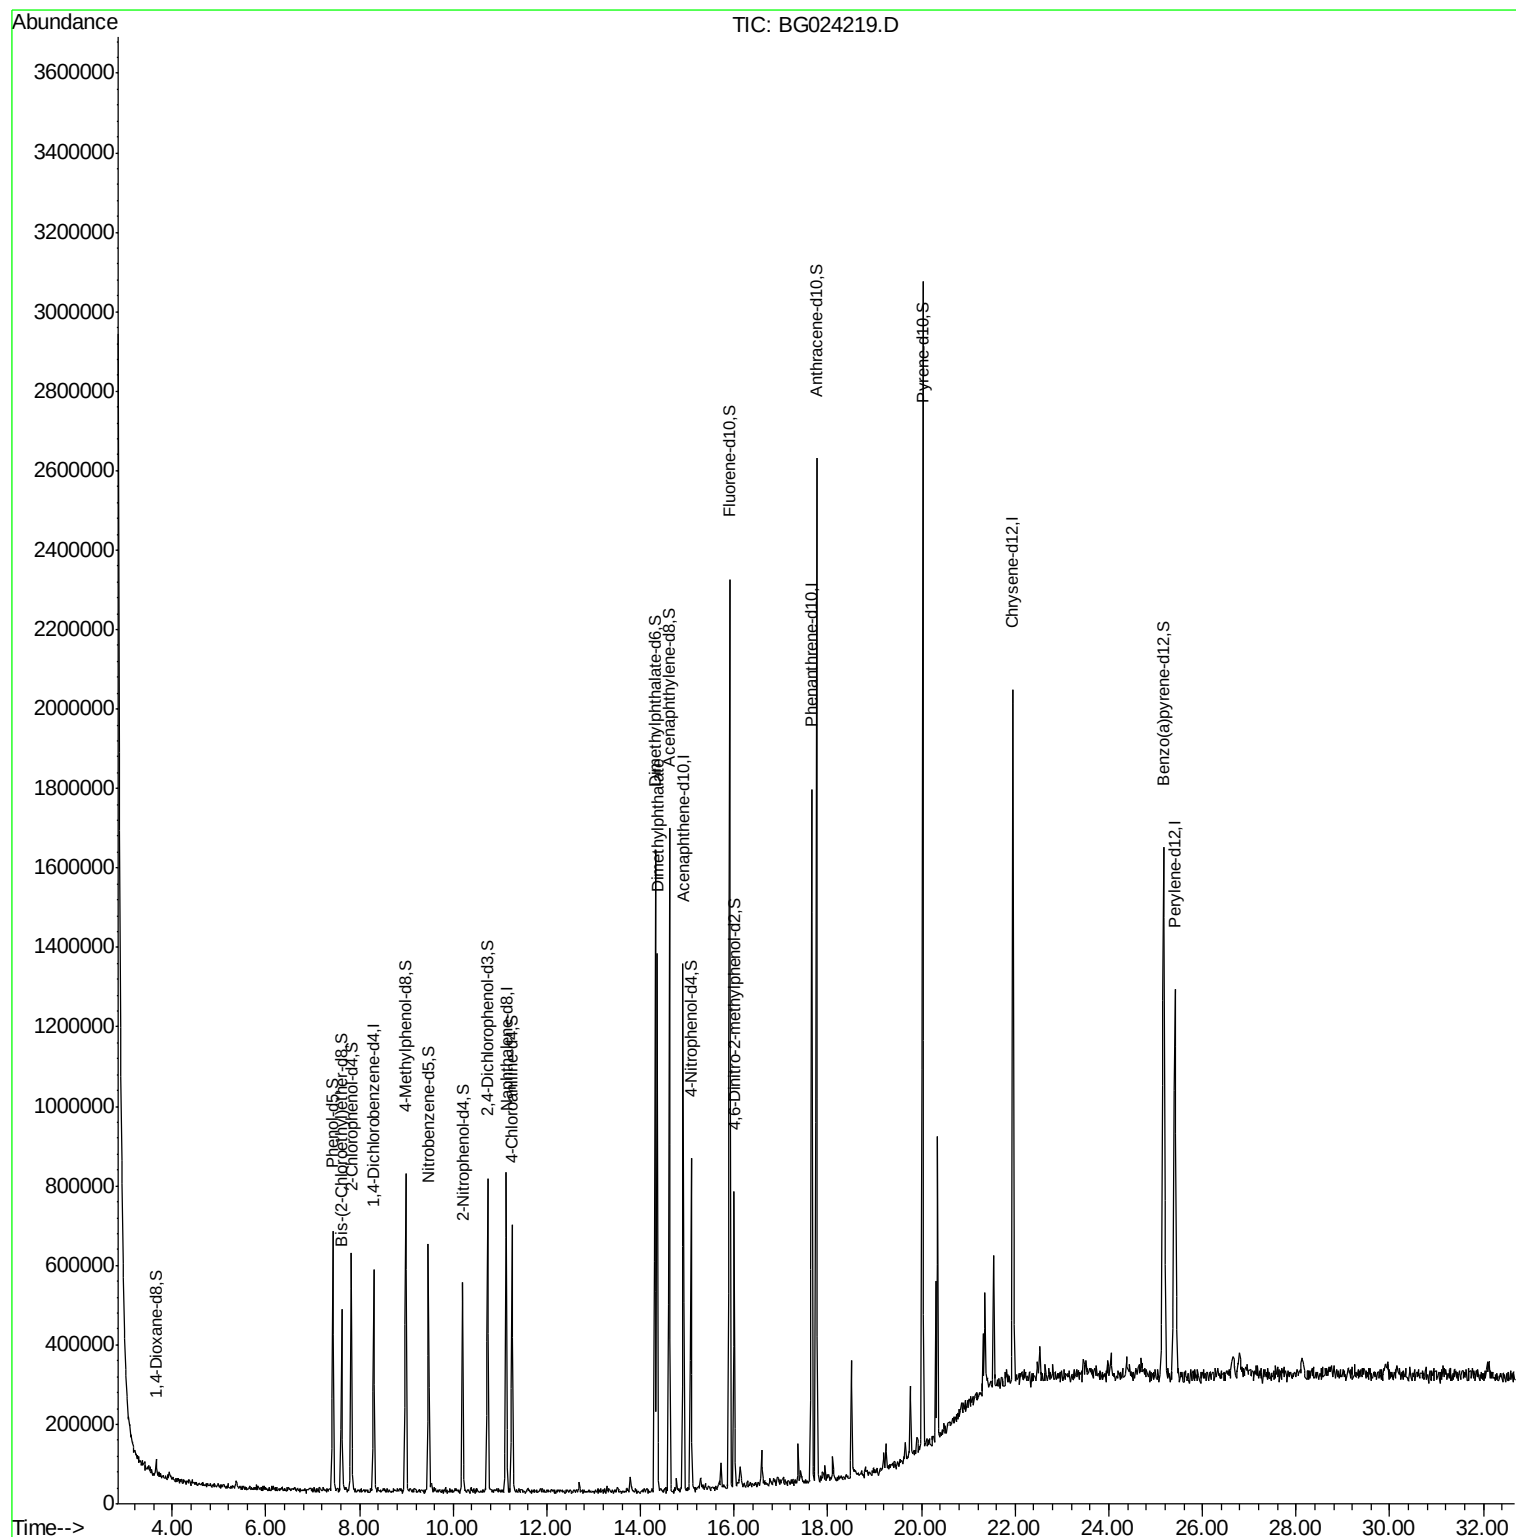

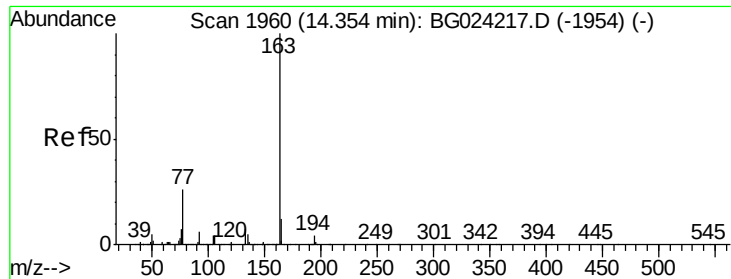

#44
 Dimethylphthalate
 Concen: 23.60 ng/ul
 RT: 14.35 min Scan# 1960
 Delta R.T. -0.00 min
 Lab File: BG024219.D
 Acq: 7 Oct 2016 4:08

Instrument :
 BNA_G
 ClientSampleId :
 BDPJ6

Tgt Ion	Ratio	Lower	Upper
163	100		
194	4.0	3.4	5.2
164	11.7	8.8	13.2

