

Data Path : Z:\HPCHEM1\BNA G\DATA\BG100717\
 Data File : BG029097.D
 Acq On : 9 Oct 2017 00:59
 Operator : SJ/JU
 Sample : I5577-01
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :

Quant Time: Oct 09 08:06:36 2017
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG100717MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 09 08:00:20 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.21	152	95206	20.00	ng/ul	0.00
2) Naphthalene-d8	11.03	136	451805	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.82	164	290231	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.56	188	651730	20.00	ng/ul	0.00
17) Chrysene-d12	21.83	240	620304	20.00	ng/ul	0.00
22) Perylene-d12	25.18	264	613770	20.00	ng/ul	0.00
System Monitoring Compounds						
7) Acenaphthylene-d8	14.52	160	74020	2.45	ng/ul	0.00
10) Fluorene-d10	15.81	176	65311	2.98	ng/ul	0.00
14) Anthracene-d10	17.66	188	104811	3.32	ng/ul	0.00
18) Pyrene-d10	19.92	212	119811	3.78	ng/ul	0.00
25) Benzo(a)pyrene-d12	24.94	264	103373	3.52	ng/ul	-0.01
Target Compounds				Ovalue		
16) Fluoranthene	19.59	202	43949	1.078	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG100717\
Data File : BG029097.D
Acq On : 9 Oct 2017 00:59
Operator : SJ/JU
Sample : I5577-01
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :

Quant Time: Oct 09 08:06:36 2017
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM-EPA-BG100717MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 09 08:00:20 2017
Response via : Initial Calibration

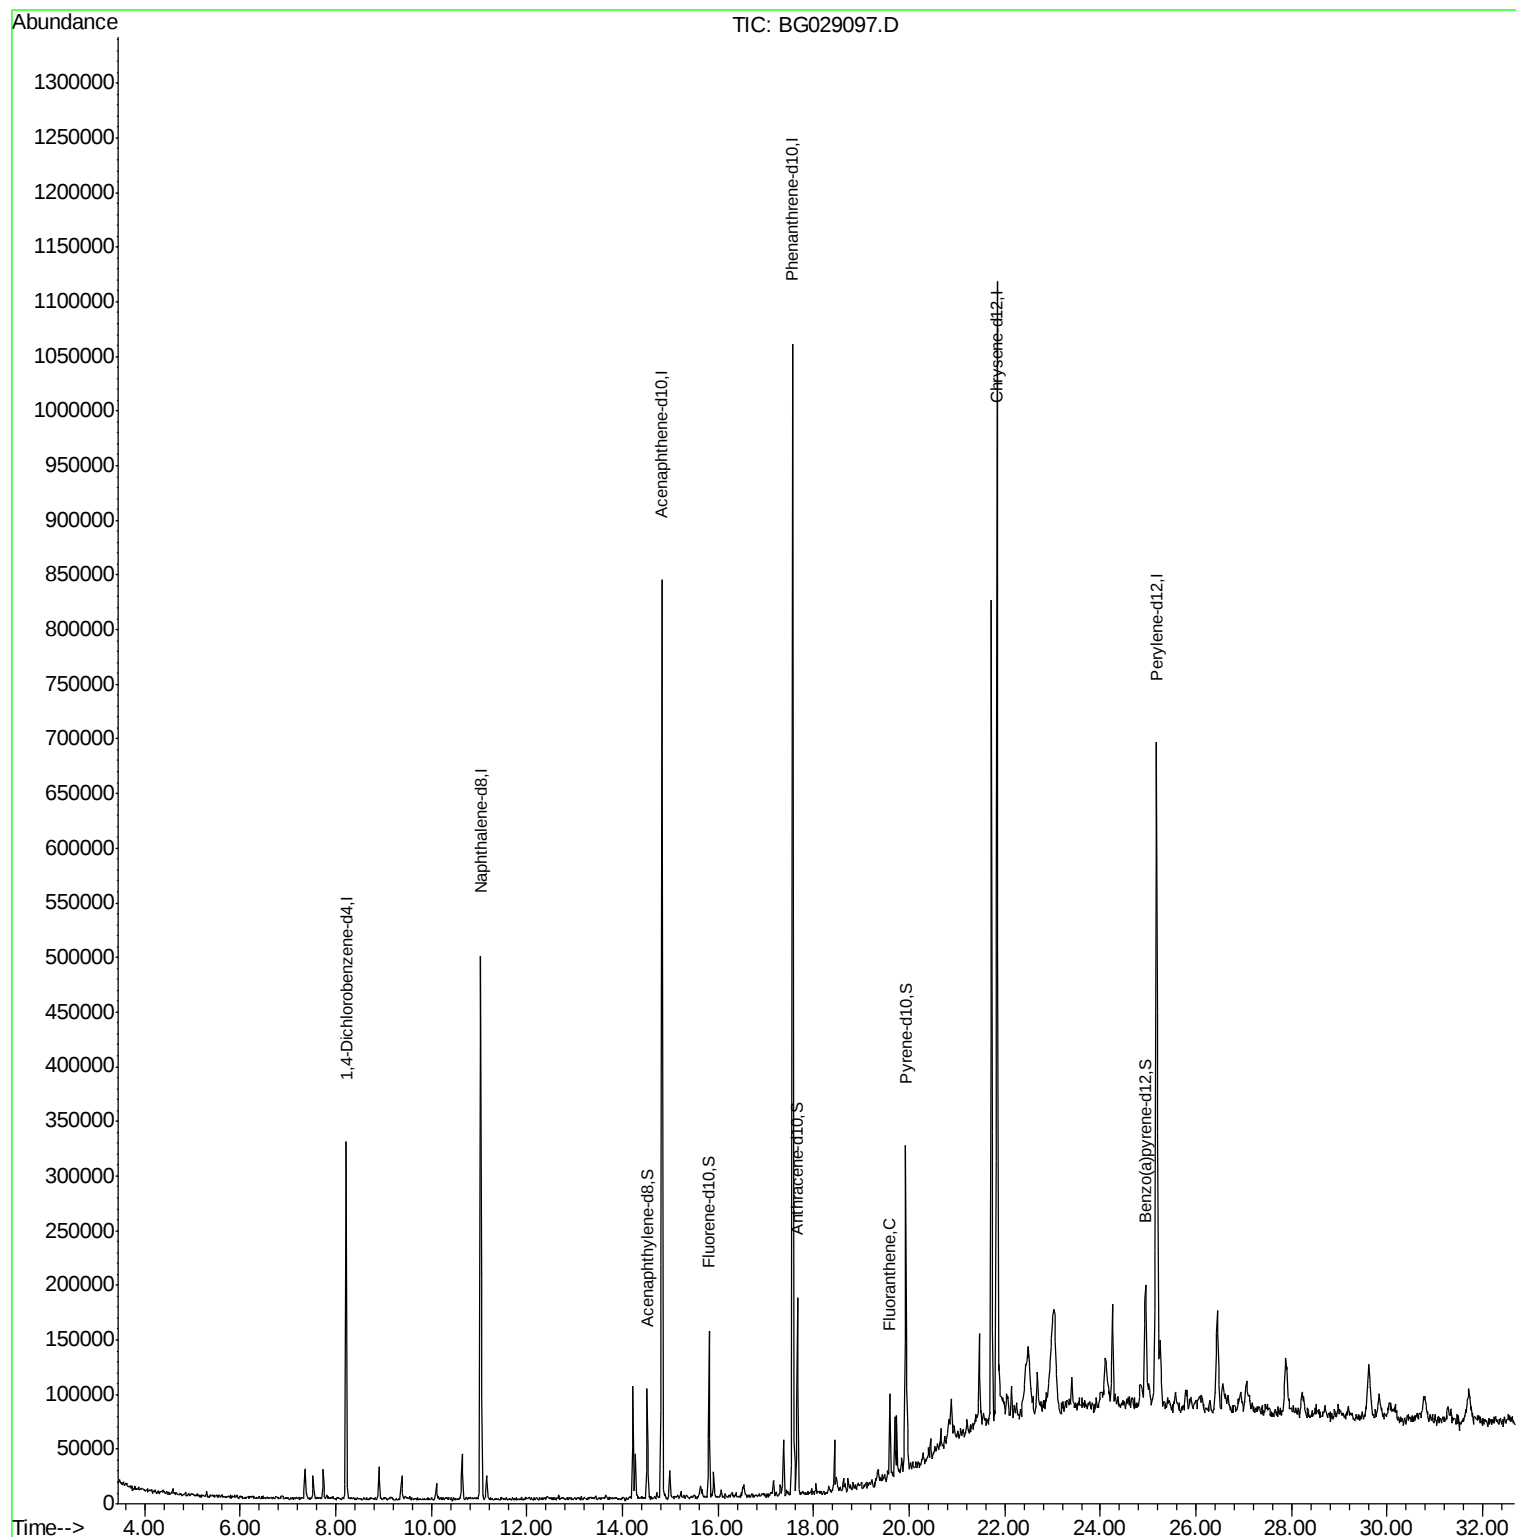

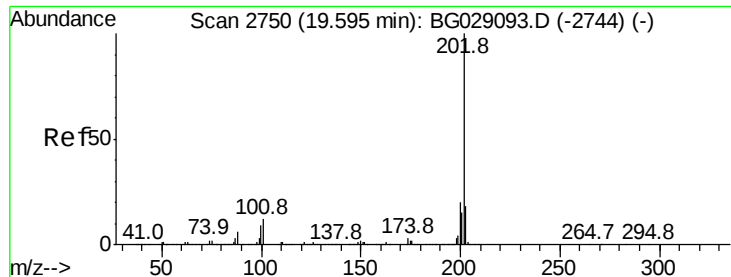

#16

Fluoranthene

Concen: 1.078 ng/ul

RT: 19.59 min Scan# 2750

Delta R.T. -0.00 min

Lab File: BG029097.D

Acq: 9 Oct 2017 00:59

Instrument :

BNA_G

ClientSampleId :


Tot Ion:202 Resp: 43949

Ion Ratio Lower Upper

202 100

101 10.7 9.9 14.9

100 8.0 7.4 11.0

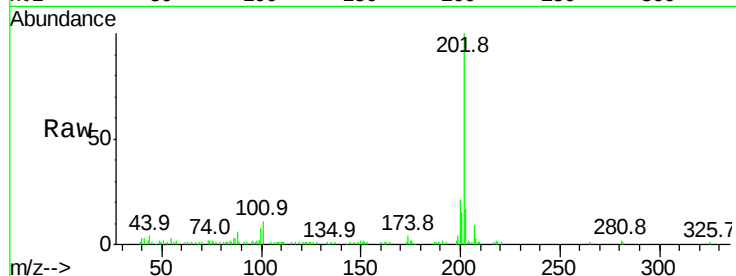

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

