
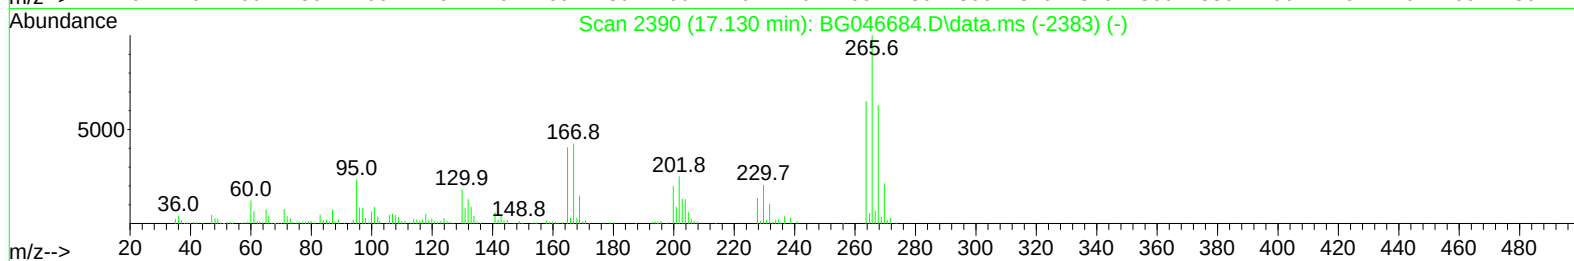
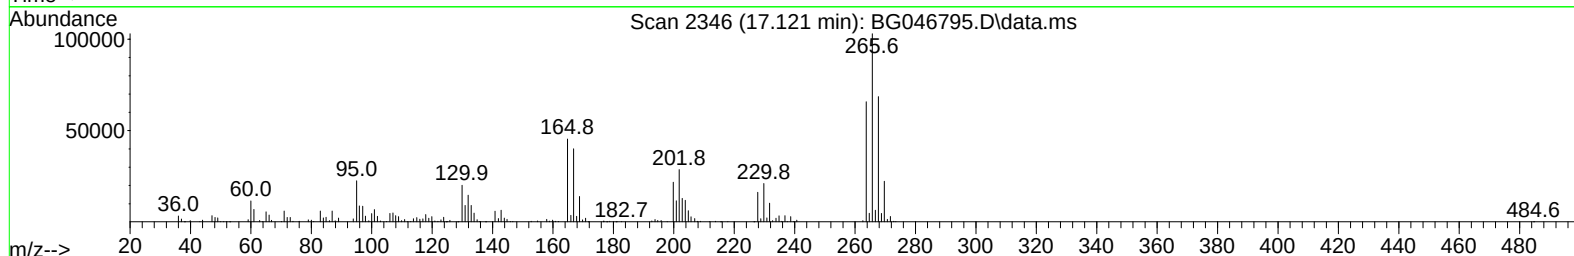


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100720\
Data File : BG046795.D
Acq On : 7 Oct 2020 8:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 08 05:27:32 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 07 11:38:17 2020
Response via : Initial Calibration

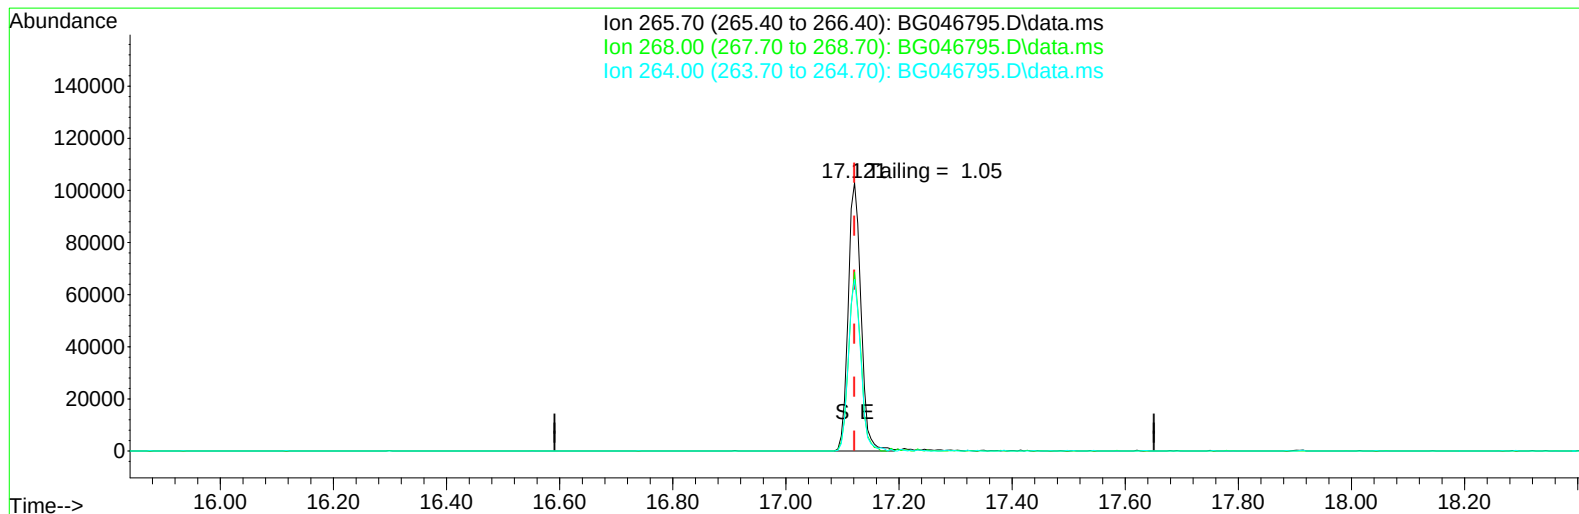

TIC: BG046795.D\data.ms

(70) Pentachlorophenol (C)




17.121min (+ 0.000) 304133.70 ng

response 162300

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.20	71.24
264.00	61.60	68.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100720\
Data File : BG046795.D
Acq On : 7 Oct 2020 8:11
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 08 05:27:32 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 07 11:38:17 2020
Response via : Initial Calibration

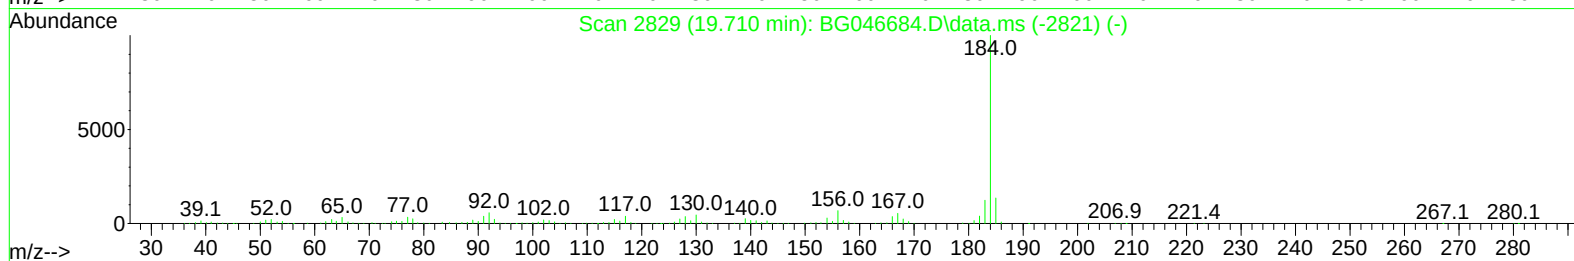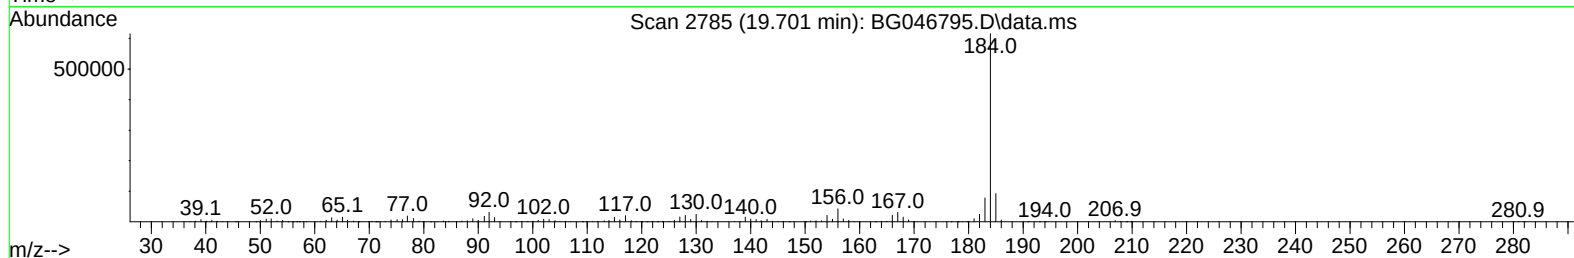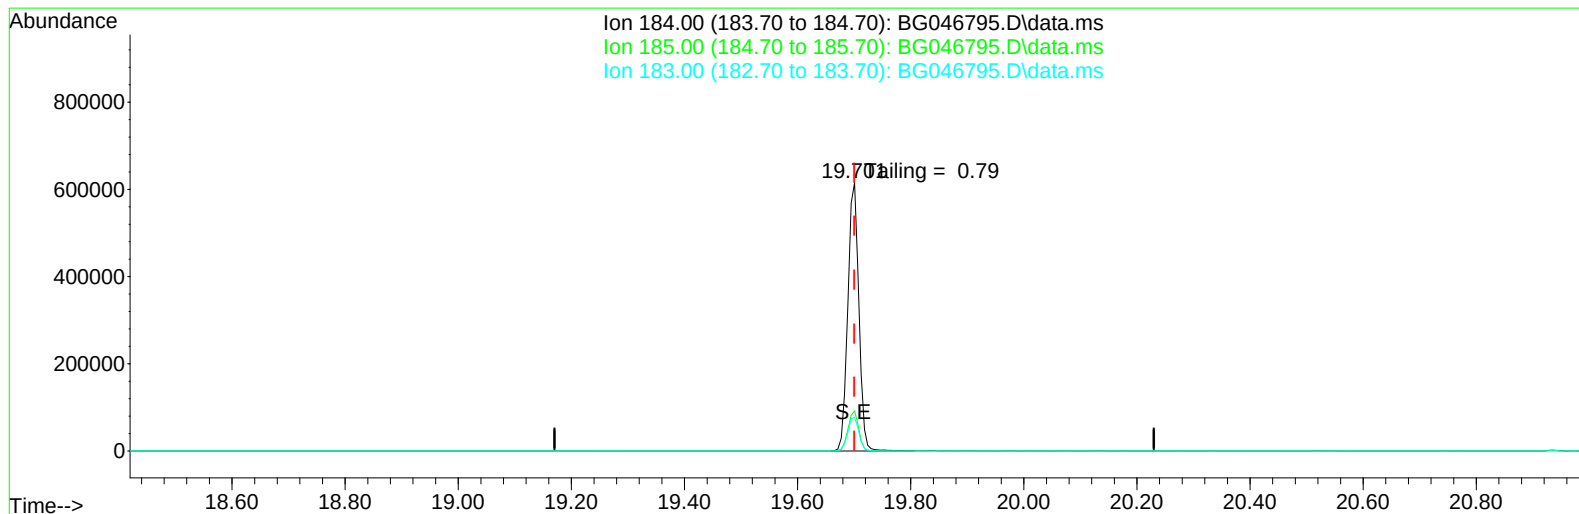

TIC: BG046795.D\data.ms

(77) Benzidine**19.701min (+ 0.000) 451273.28 ng****response 834640**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.96
183.00	13.20	12.74
0.00	0.00	0.00