

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG100720\  
 Data File : BG046797.D  
 Acq On : 7 Oct 2020 10:12  
 Operator : CG/JU  
 Sample : PB132101BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_G  
 ClientSampleId :  
 PB132101BL

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : ON Filtering: 5  
 Sampling : 1 Min Area: 3 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG092220.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG046797.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.671       | 389           | 397         | 407          | rBV      | 1311785        | 2043570       | 32.23%          | 8.728%        |
| 2         | 7.257       | 659           | 667         | 679          | rBV      | 1255607        | 2151401       | 33.93%          | 9.188%        |
| 3         | 8.109       | 804           | 812         | 819          | rBV2     | 229601         | 390004        | 6.15%           | 1.666%        |
| 4         | 9.273       | 1000          | 1010        | 1017         | rBV      | 849114         | 1495123       | 23.58%          | 6.386%        |
| 5         | 10.924      | 1280          | 1291        | 1299         | rBV      | 300485         | 535531        | 8.45%           | 2.287%        |
| 6         | 13.362      | 1698          | 1706        | 1712         | rBV      | 2191791        | 3374348       | 53.22%          | 14.412%       |
| 7         | 14.731      | 1932          | 1939        | 1947         | rVB2     | 509209         | 783104        | 12.35%          | 3.345%        |
| 8         | 16.217      | 2184          | 2192        | 2206         | rBV      | 1796065        | 2704155       | 42.65%          | 11.549%       |
| 9         | 17.475      | 2399          | 2406        | 2413         | rBV      | 663838         | 1011427       | 15.95%          | 4.320%        |
| 10        | 20.083      | 2843          | 2850        | 2855         | rBV      | 4767713        | 6340122       | 100.00%         | 27.078%       |
| 11        | 21.752      | 3127          | 3134        | 3141         | rBV      | 791860         | 1310348       | 20.67%          | 5.596%        |
| 12        | 25.025      | 3680          | 3691        | 3702         | rBV2     | 455088         | 1274961       | 20.11%          | 5.445%        |




Sum of corrected areas: 23414094

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG100720\  
Data File : BG046797.D  
Acq On : 7 Oct 2020 10:12  
Operator : CG/JU  
Sample : PB132101BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB132101BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG092220.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L  
TIC Integration Parameters: LSCINT.P

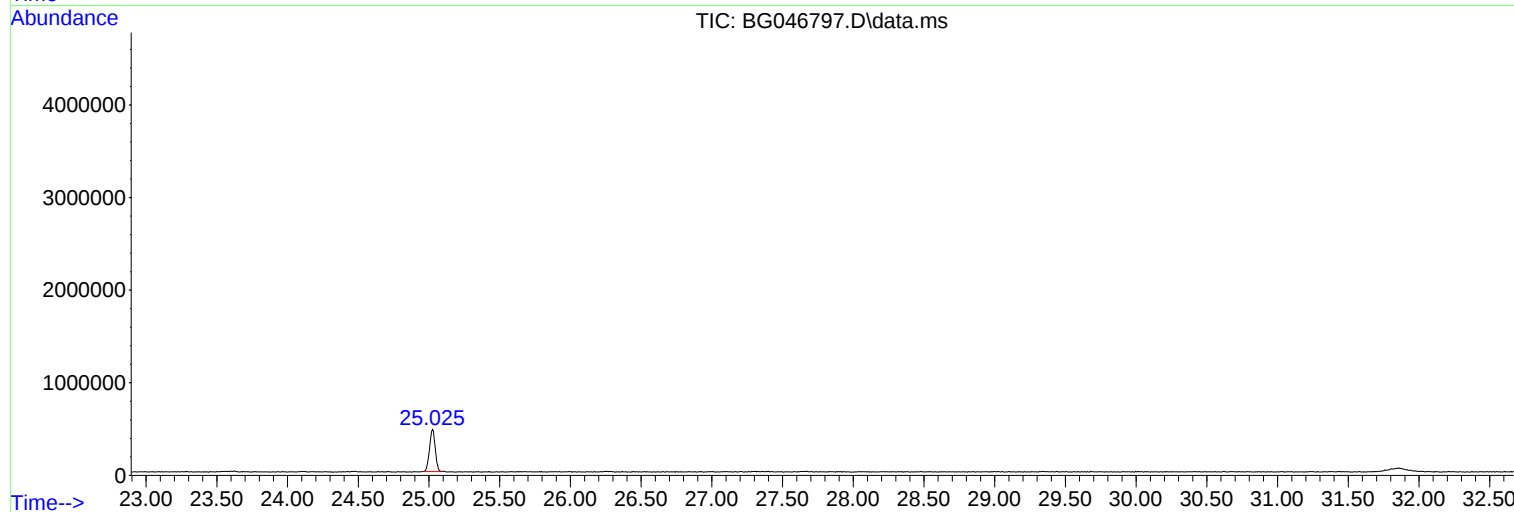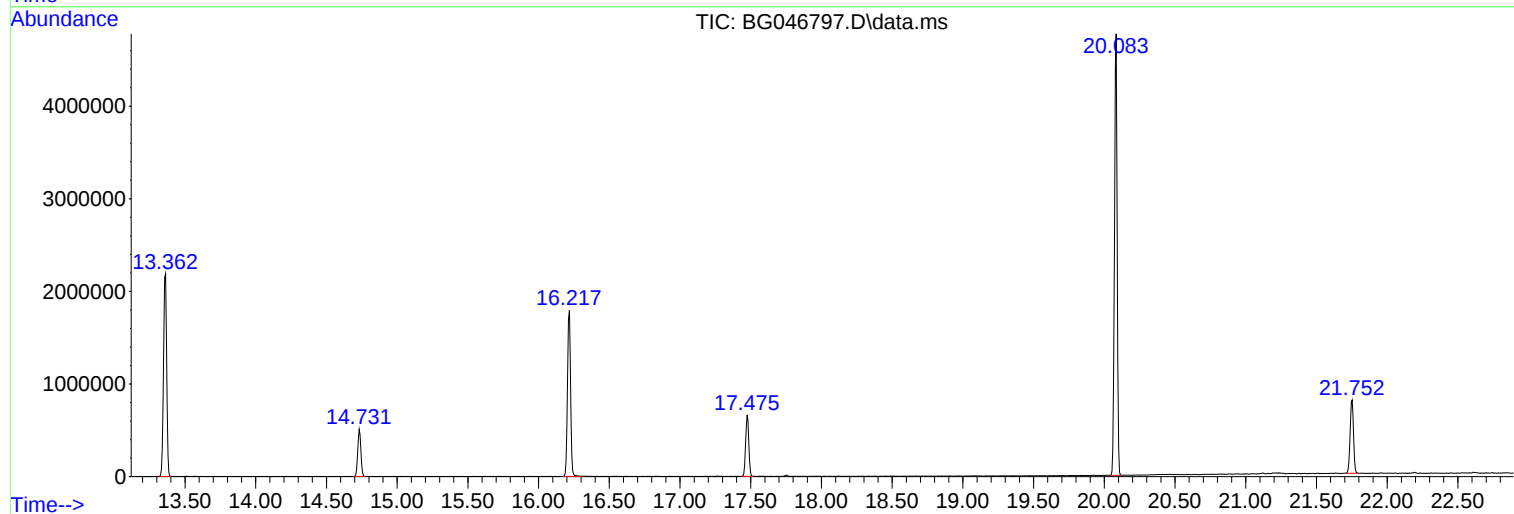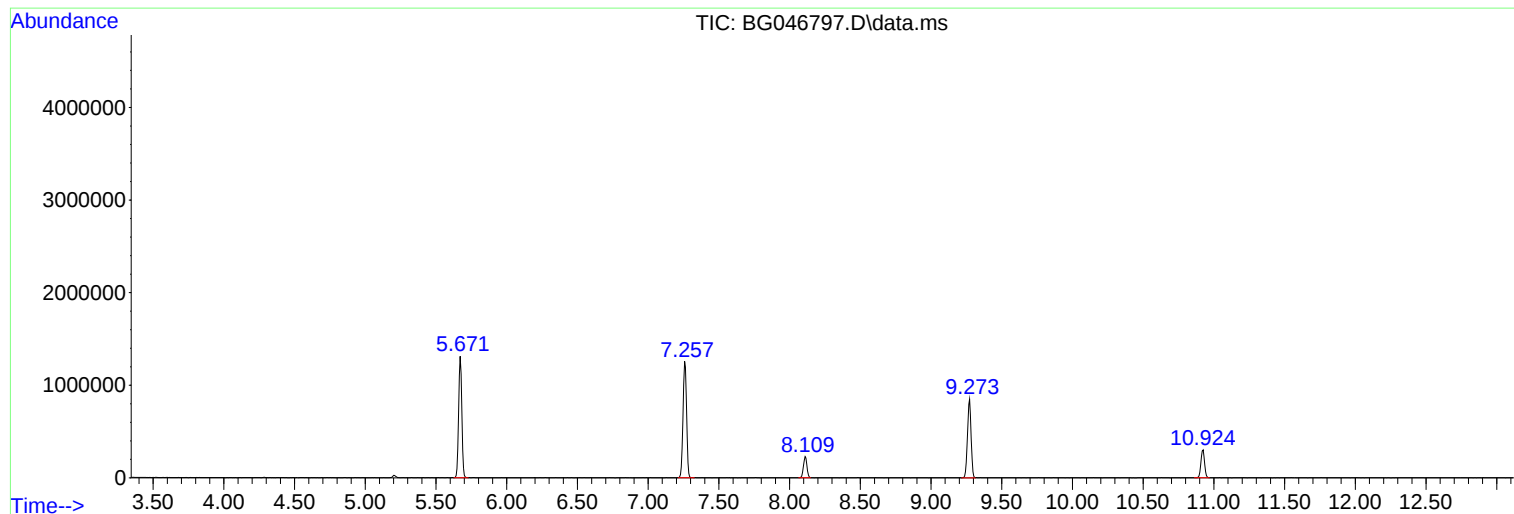

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG100720\  
Data File : BG046797.D  
Acq On : 7 Oct 2020 10:12  
Operator : CG/JU  
Sample : PB132101BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB132101BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG092220.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG100720\  
Data File : BG046797.D  
Acq On : 7 Oct 2020 10:12  
Operator : CG/JU  
Sample : PB132101BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_G  
ClientSampleId :  
PB132101BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_G\METHODS\8270-BG092220.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST11.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|