
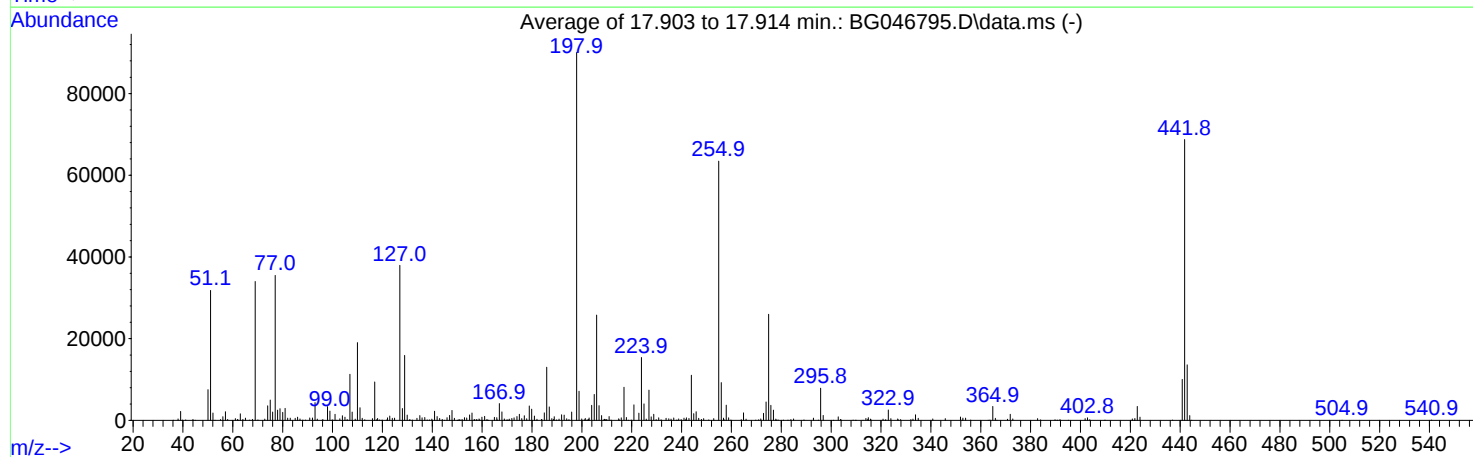


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100720\
 Data File : BG046795.D
 Acq On : 7 Oct 2020 8:11
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 07 11:38:17 2020

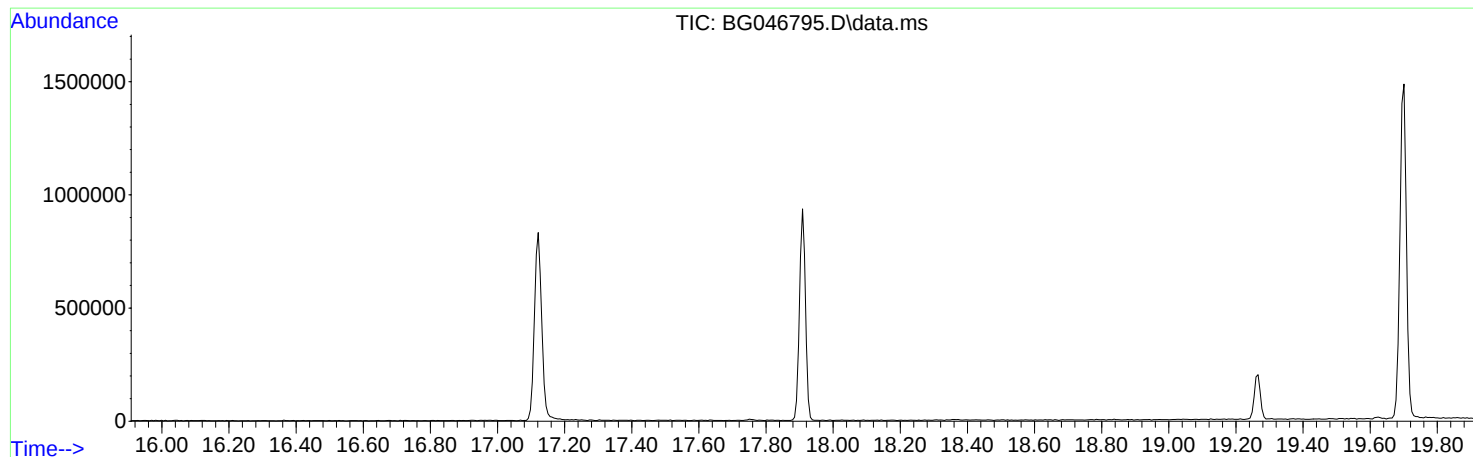

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.3	31813	PASS
68	69	0.00	2	0.7	246	PASS
69	198	0.00	100	37.8	34019	PASS
70	69	0.00	2	0.3	119	PASS
127	198	10	80	42.1	37955	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	90056	PASS
199	198	5	9	7.9	7116	PASS
275	198	10	60	28.9	25984	PASS
365	198	1	100	3.8	3392	PASS
441	198	0.01	100	11.1	10019	PASS
442	198	50	100	76.3	68744	PASS
443	442	15	24	19.8	13599	PASS