
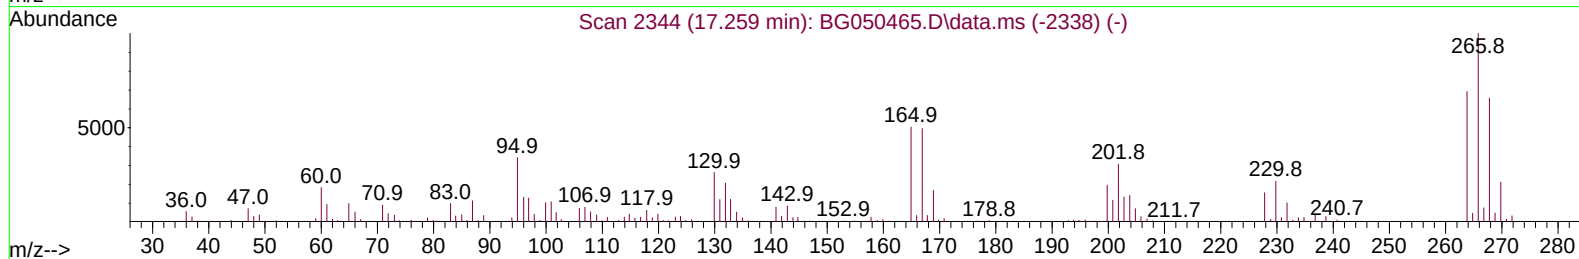
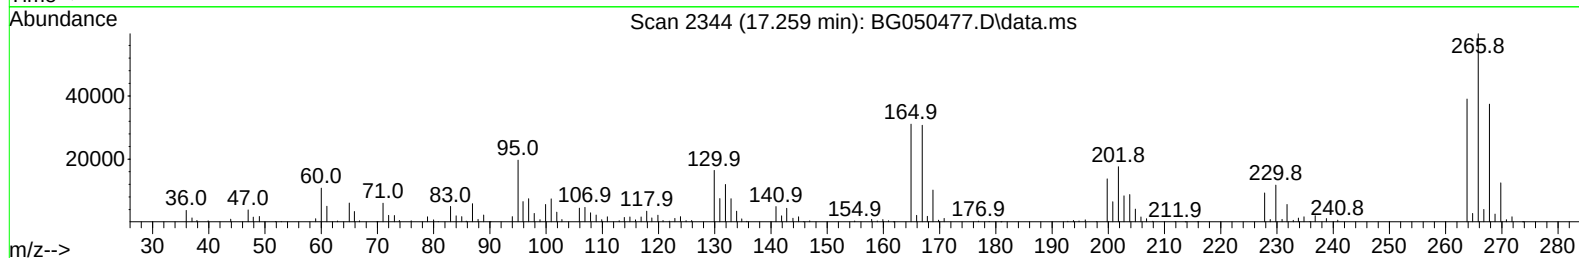


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100721\
Data File : BG050477.D
Acq On : 7 Oct 2021 9:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 13:13:11 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 06 15:51:01 2021
Response via : Initial Calibration

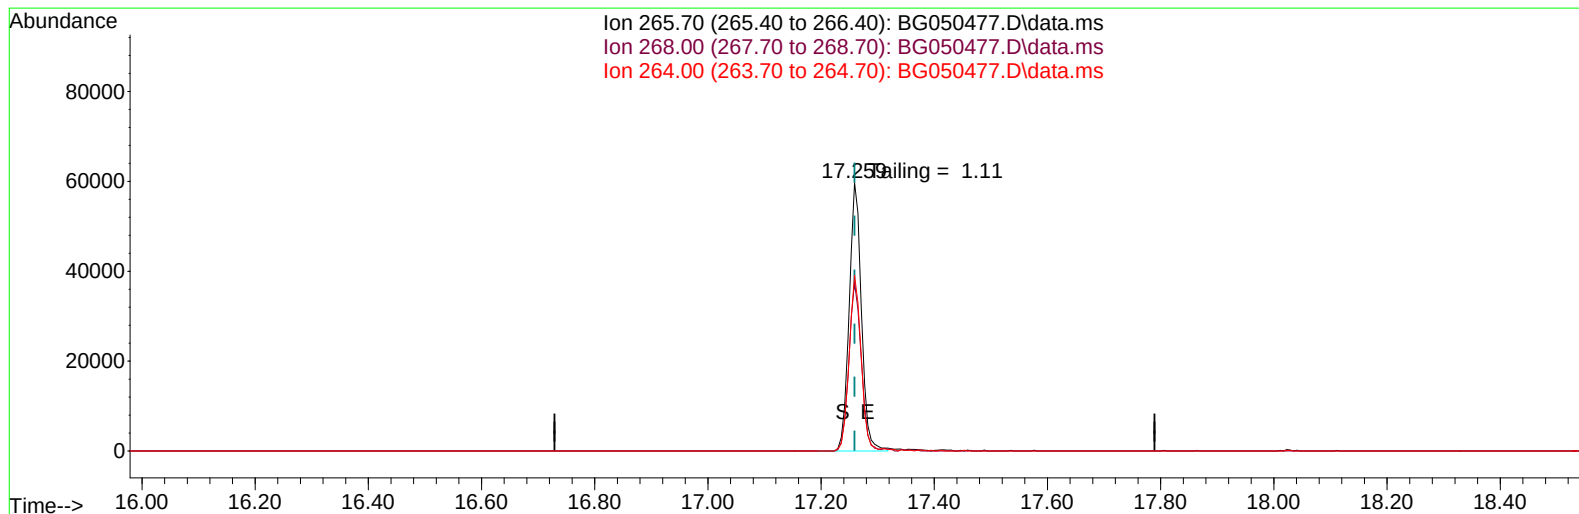

TIC: BG050477.D\data.ms

(70) Pentachlorophenol (C)




17.259min (+ 0.000) 17235.74 ng

response 90718

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	62.66
264.00	61.30	65.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100721\
Data File : BG050477.D
Acq On : 7 Oct 2021 9:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 13:13:11 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 06 15:51:01 2021
Response via : Initial Calibration

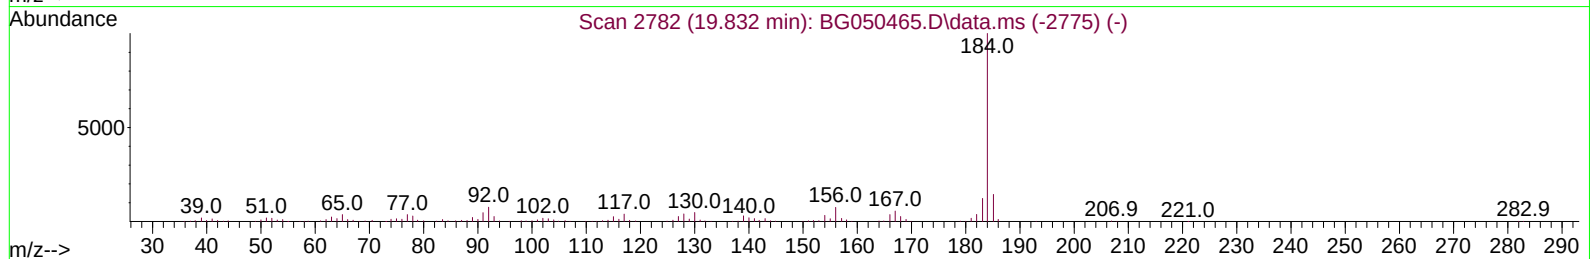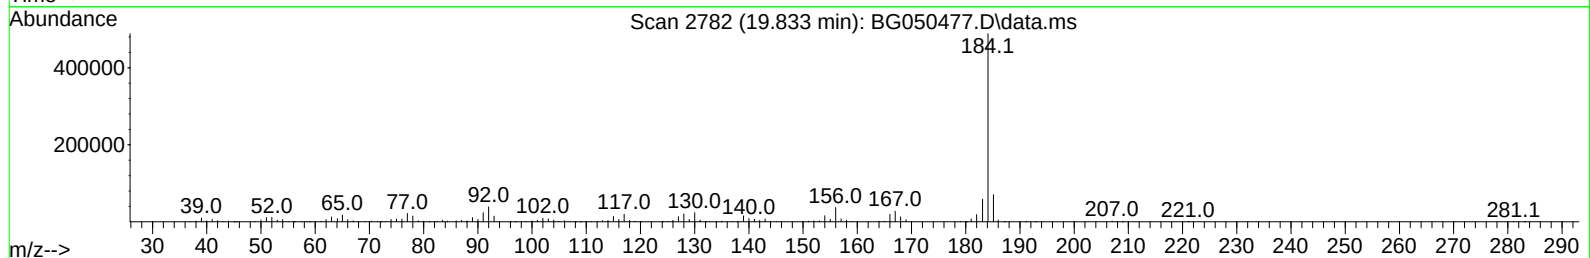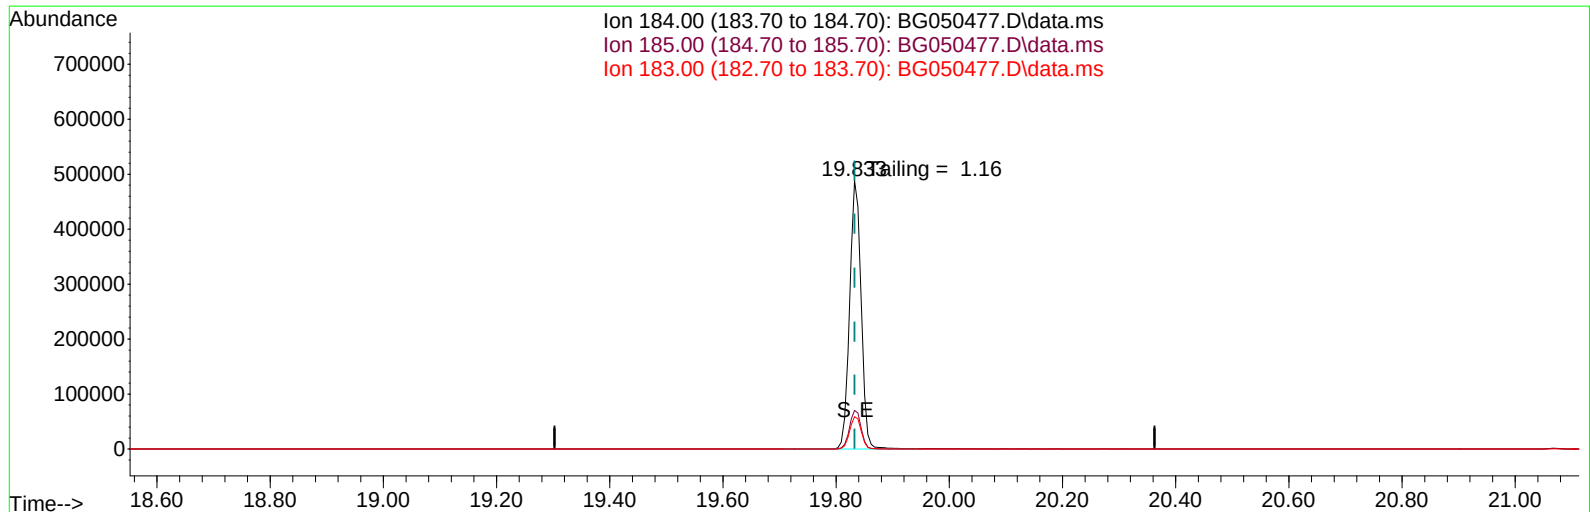

TIC: BG050477.D\data.ms

(77) Benzidine

19.833min (+ 0.000) 0.00 ng

response 690577

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.38
183.00	11.70	12.07
0.00	0.00	0.00