
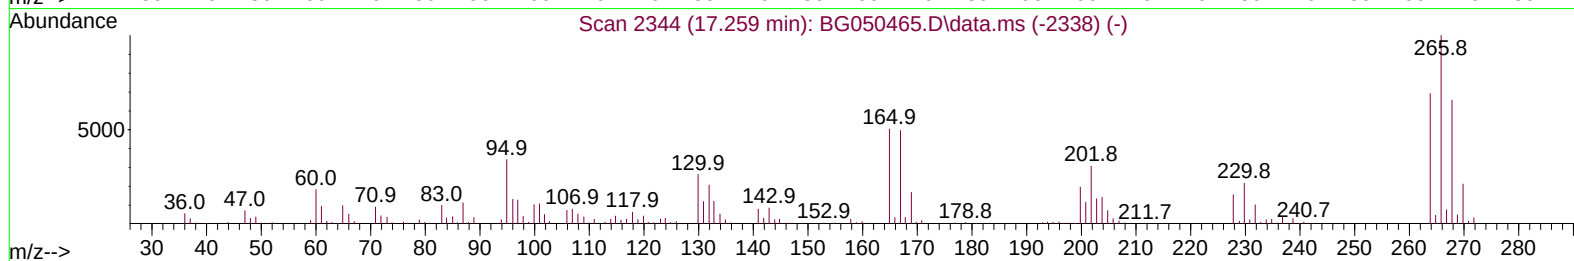
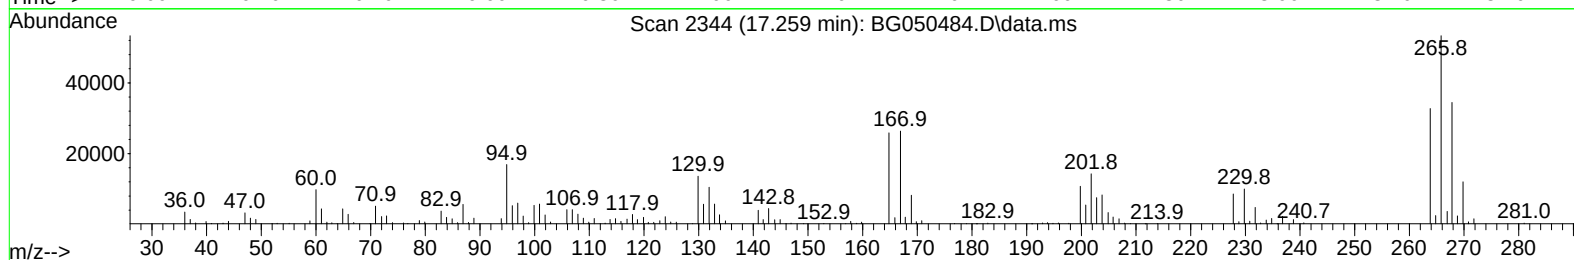


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100721\
Data File : BG050484.D
Acq On : 7 Oct 2021 15:26
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 17:51:09 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 06 15:51:01 2021
Response via : Initial Calibration

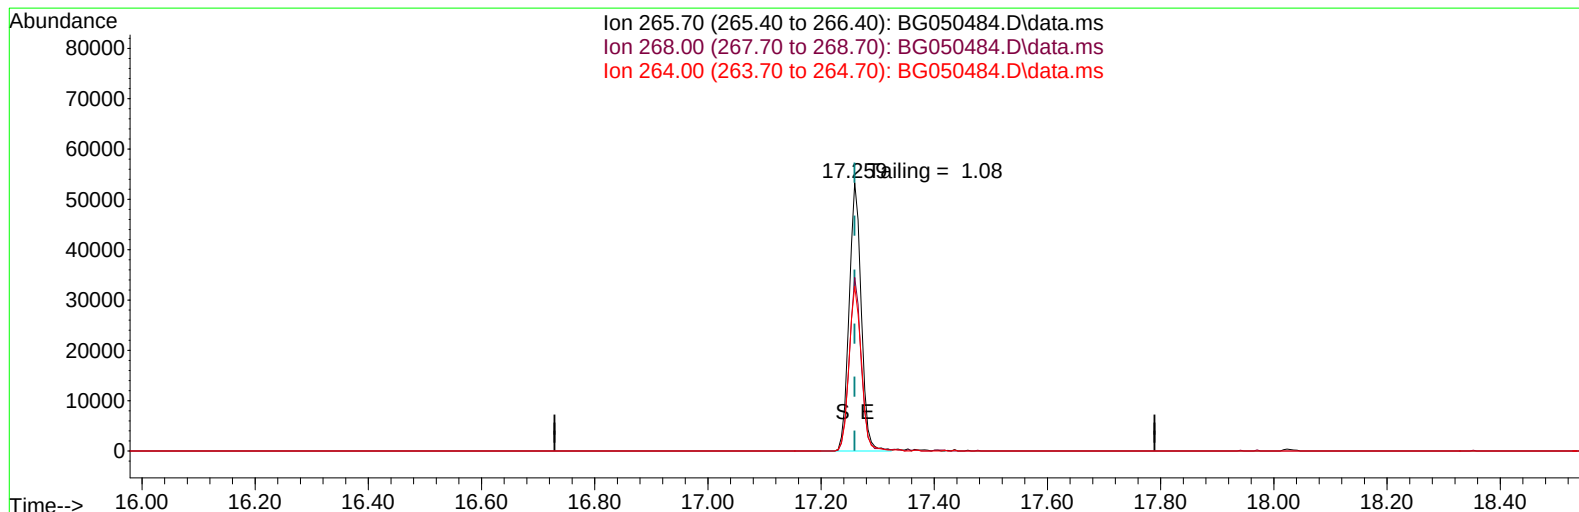

TIC: BG050484.D\data.ms

(70) Pentachlorophenol (C)




17.259min (+ 0.001) 27469.93 ng

response 79409

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	64.66
264.00	61.30	61.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100721\
 Data File : BG050484.D
 Acq On : 7 Oct 2021 15:26
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 07 17:51:09 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 06 15:51:01 2021
 Response via : Initial Calibration

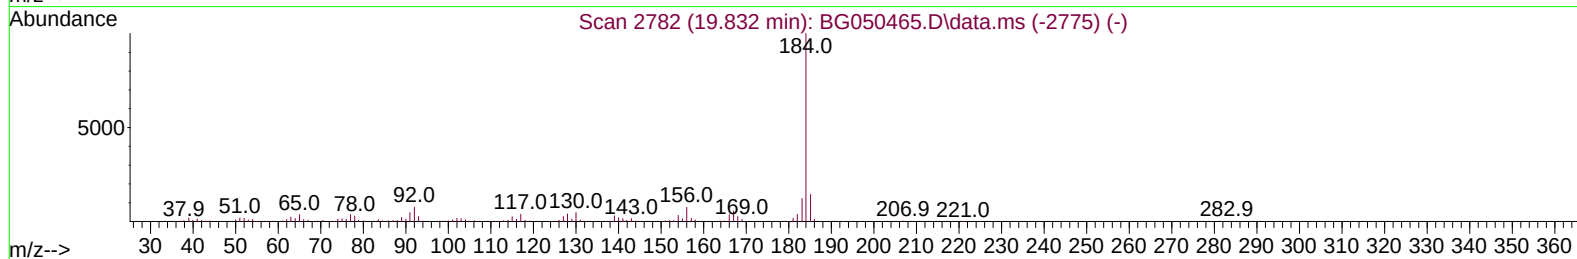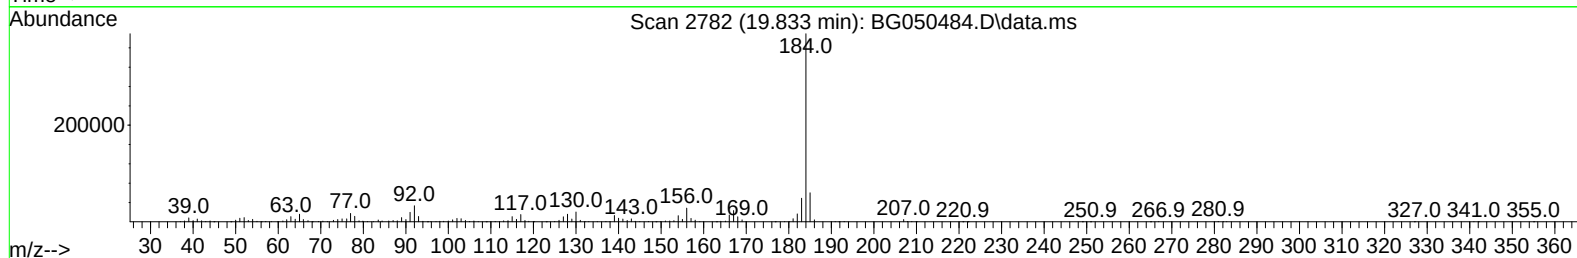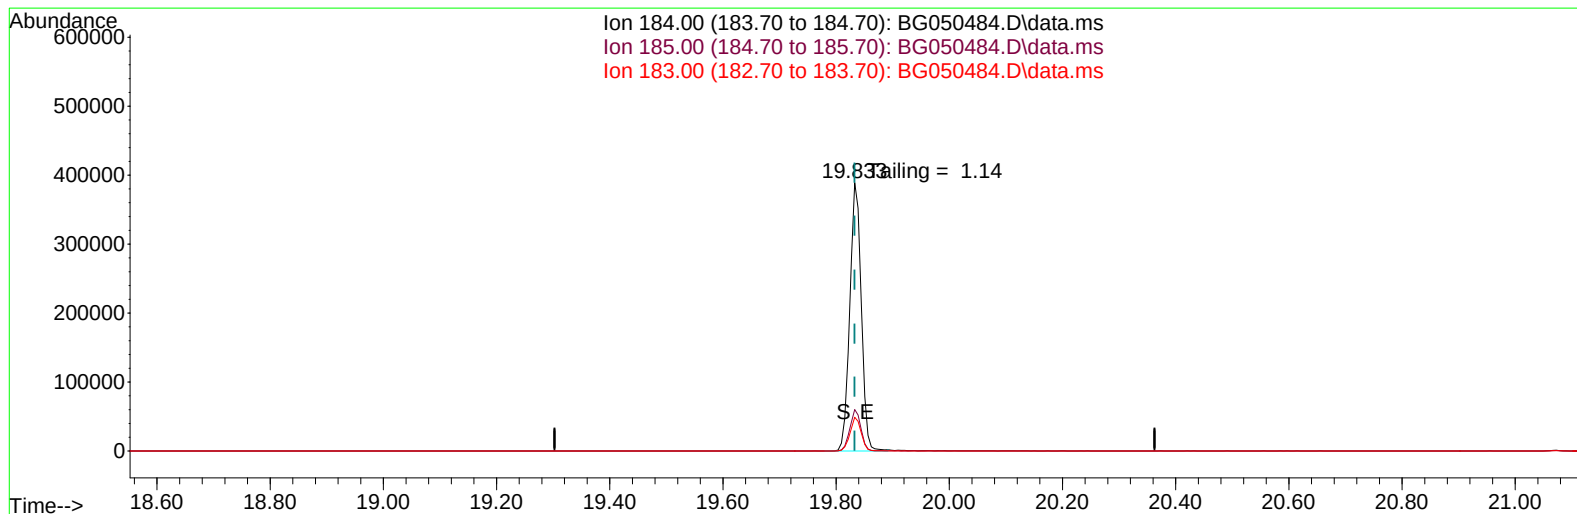

TIC: BG050484.D\data.ms

(77) Benzidine**19.833min (+ 0.001) 201614.75 ng****response 548904**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	15.49
183.00	11.70	12.57
0.00	0.00	0.00