

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100721\
 Data File : BG050487.D
 Acq On : 7 Oct 2021 17:40
 Operator : CG/JU
 Sample : M4113-03
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 TP-2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BG050487.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.794	384	392	401	rBV	772663	1252541	47.51%	9.476%
2	7.398	654	665	676	rBV	747139	1357125	51.48%	10.267%
3	8.262	805	812	825	rVB	151634	273545	10.38%	2.069%
4	9.431	1001	1011	1019	rBV	471511	855389	32.45%	6.471%
5	10.829	1242	1249	1259	rBV2	52376	91870	3.48%	0.695%
6	11.082	1283	1292	1301	rVB	199826	378427	14.35%	2.863%
7	13.502	1696	1704	1712	rBV	1056449	1674411	63.51%	12.667%
8	14.877	1931	1938	1947	rVB	317084	507387	19.25%	3.838%
9	16.358	2183	2190	2203	rVB	867902	1319332	50.04%	9.981%
10	17.615	2394	2404	2411	rBV	408378	651877	24.73%	4.931%
11	18.473	2546	2550	2563	rBV	129632	220476	8.36%	1.668%
12	19.736	2759	2765	2779	rBV3	60706	120163	4.56%	0.909%
13	20.206	2839	2845	2851	rBV	2023676	2636384	100.00%	19.944%
14	21.023	2976	2984	2991	rVB6	20147	50003	1.90%	0.378%
15	21.522	3064	3069	3080	rVB3	118198	214359	8.13%	1.622%
16	21.616	3082	3085	3096	rVB	24269	38201	1.45%	0.289%
17	21.916	3130	3136	3143	rVB	402530	699139	26.52%	5.289%
18	22.762	3274	3280	3290	rVB6	31885	92516	3.51%	0.700%
19	23.679	3431	3436	3441	rVB2	32847	63785	2.42%	0.483%
20	25.330	3706	3717	3730	rVB2	238468	721780	27.38%	5.460%




Sum of corrected areas: 13218710

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100721\
Data File : BG050487.D
Acq On : 7 Oct 2021 17:40
Operator : CG/JU
Sample : M4113-03
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

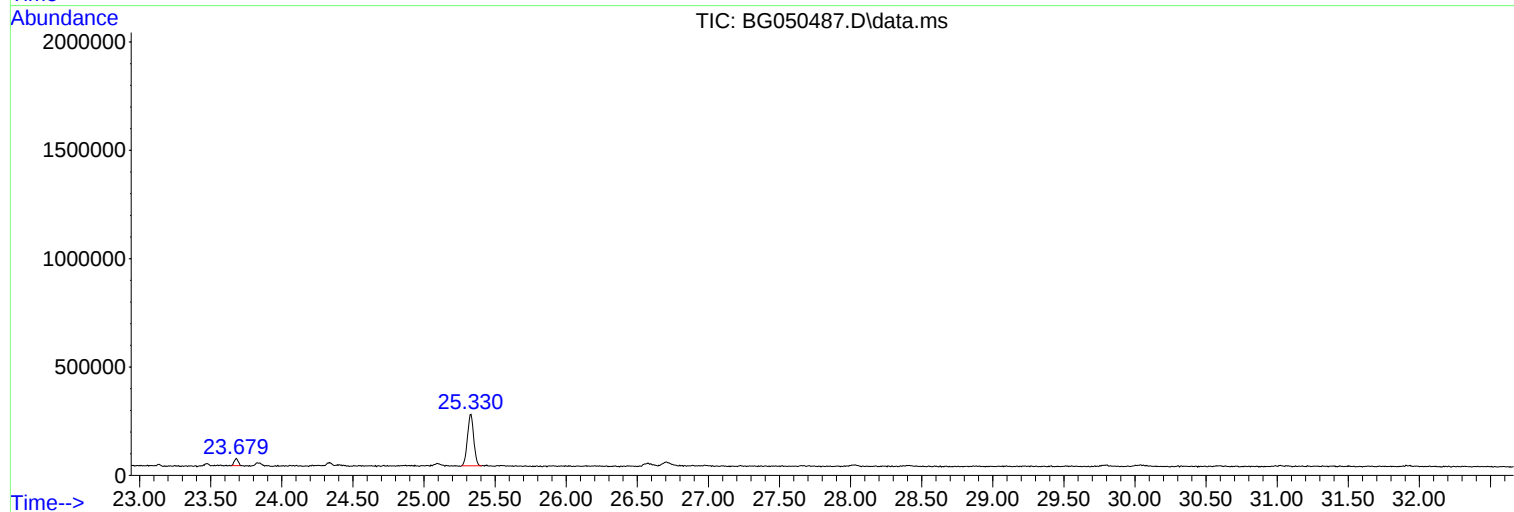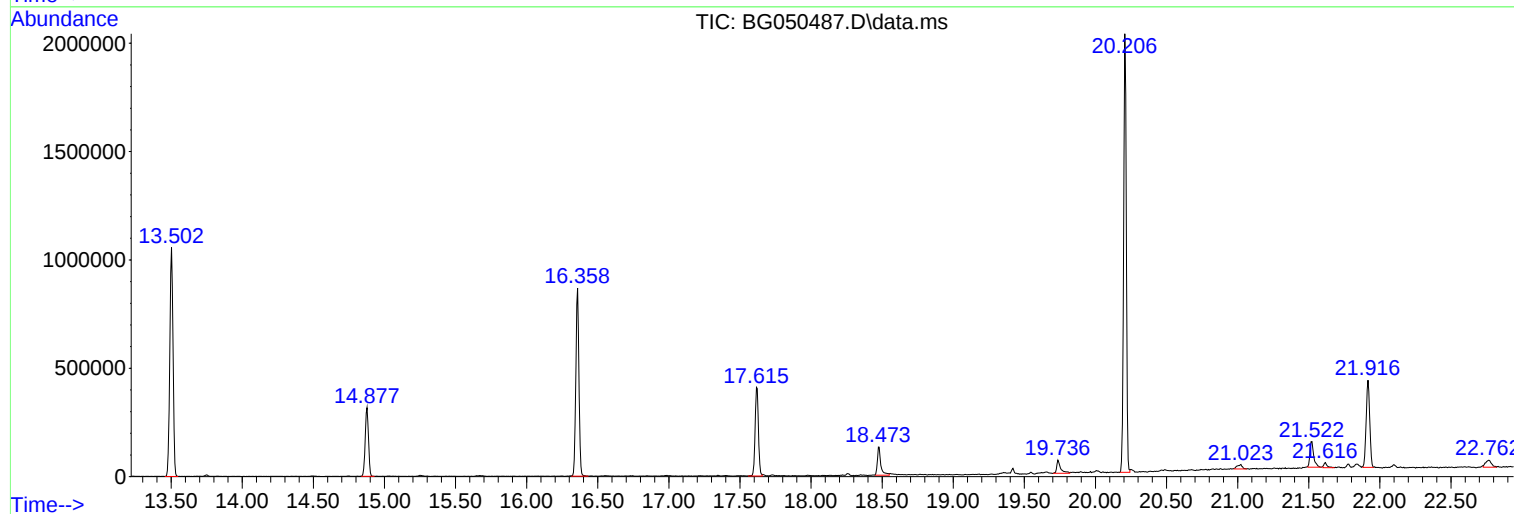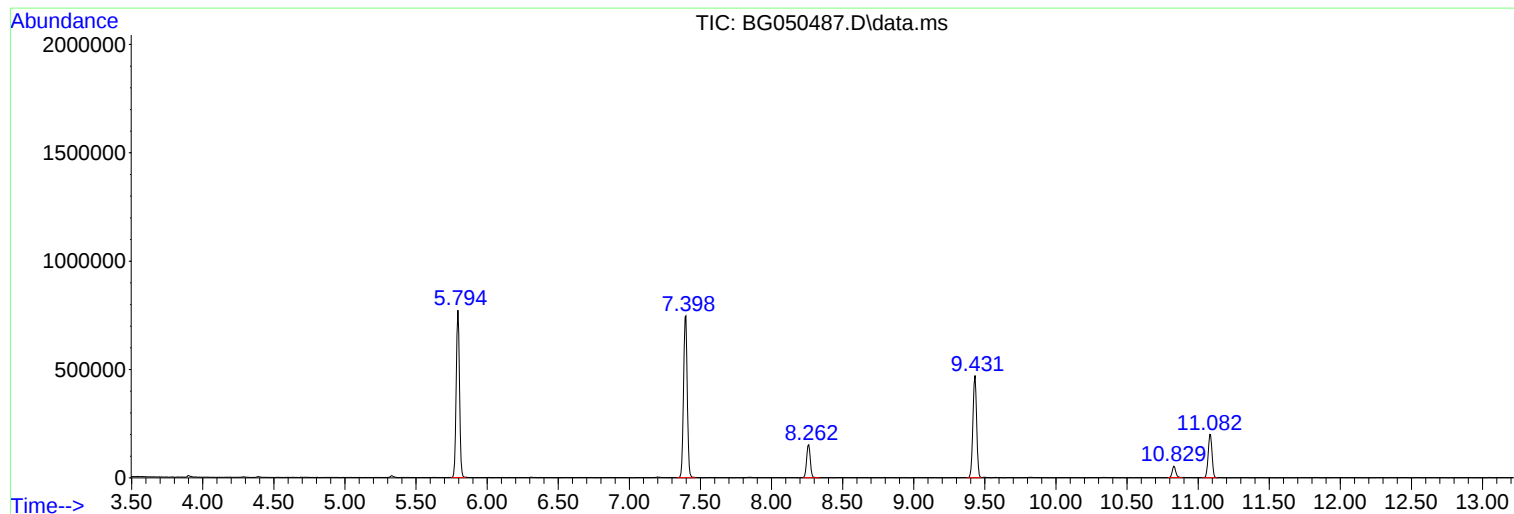

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100721\
Data File : BG050487.D
Acq On : 7 Oct 2021 17:40
Operator : CG/JU
Sample : M4113-03
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100721\
Data File : BG050487.D
Acq On : 7 Oct 2021 17:40
Operator : CG/JU
Sample : M4113-03
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
TP-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
