
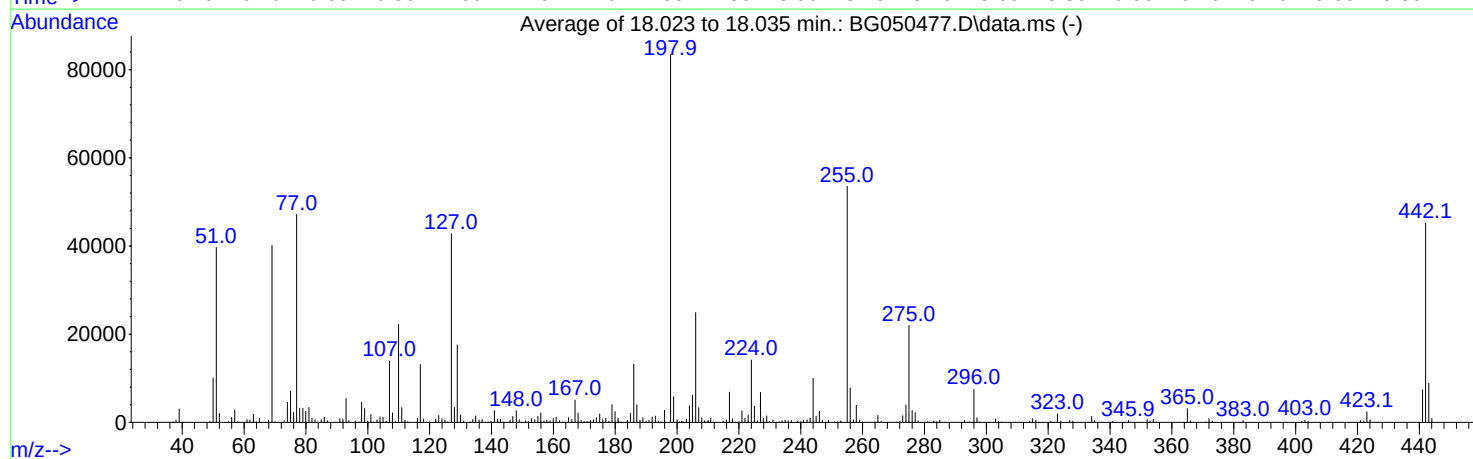


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100721\
 Data File : BG050477.D
 Acq On : 7 Oct 2021 9:51
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 06 15:51:01 2021

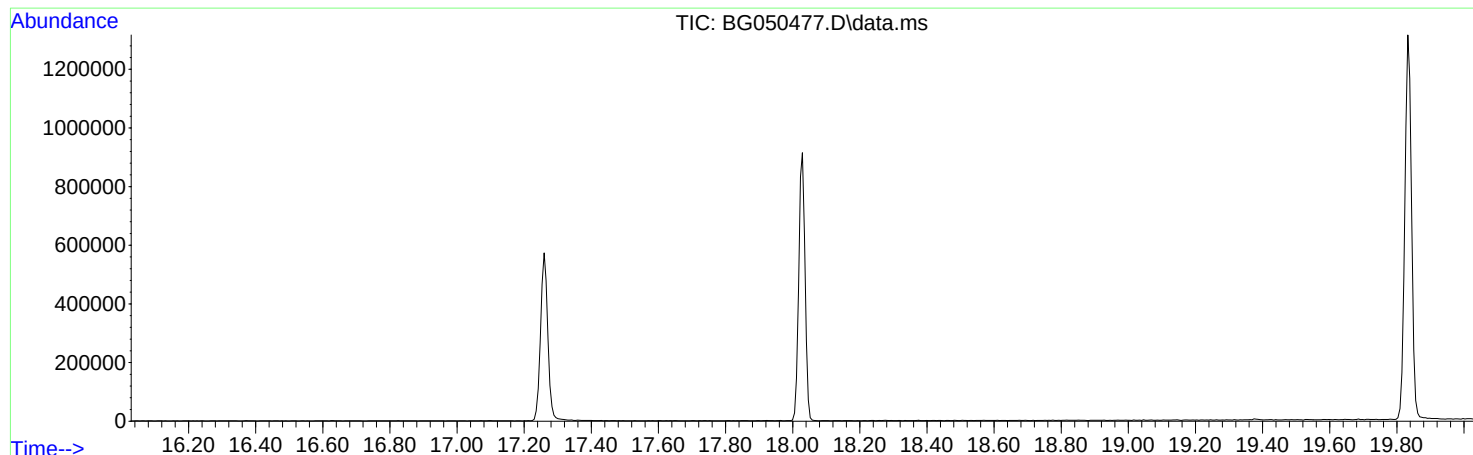




AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.5	39653	PASS
68	69	0.00	2	1.4	553	PASS
69	198	0.00	100	48.1	40133	PASS
70	69	0.00	2	0.4	158	PASS
127	198	10	80	51.3	42789	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	83435	PASS
199	198	5	9	7.0	5803	PASS
275	198	10	60	26.4	21987	PASS
365	198	1	100	3.8	3130	PASS
441	198	0.01	100	8.8	7366	PASS
442	442	50	100	100.0	45157	PASS
443	442	15	24	19.6	8861	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100721\
Data File : BG050477.D
Acq On : 7 Oct 2021 9:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 07 13:13:11 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 06 15:51:01 2021
Response via : Initial Calibration

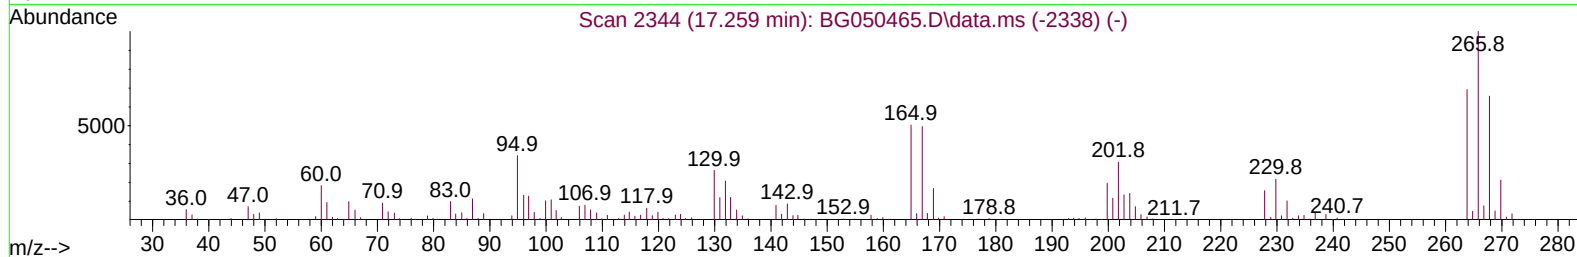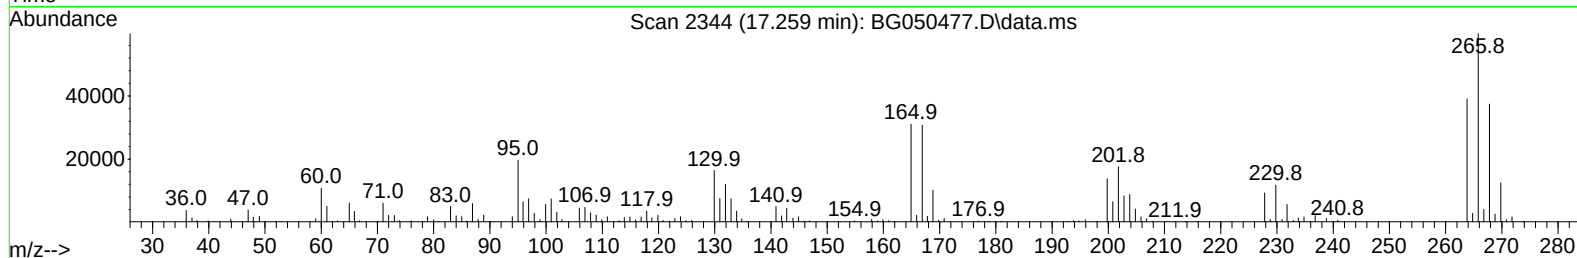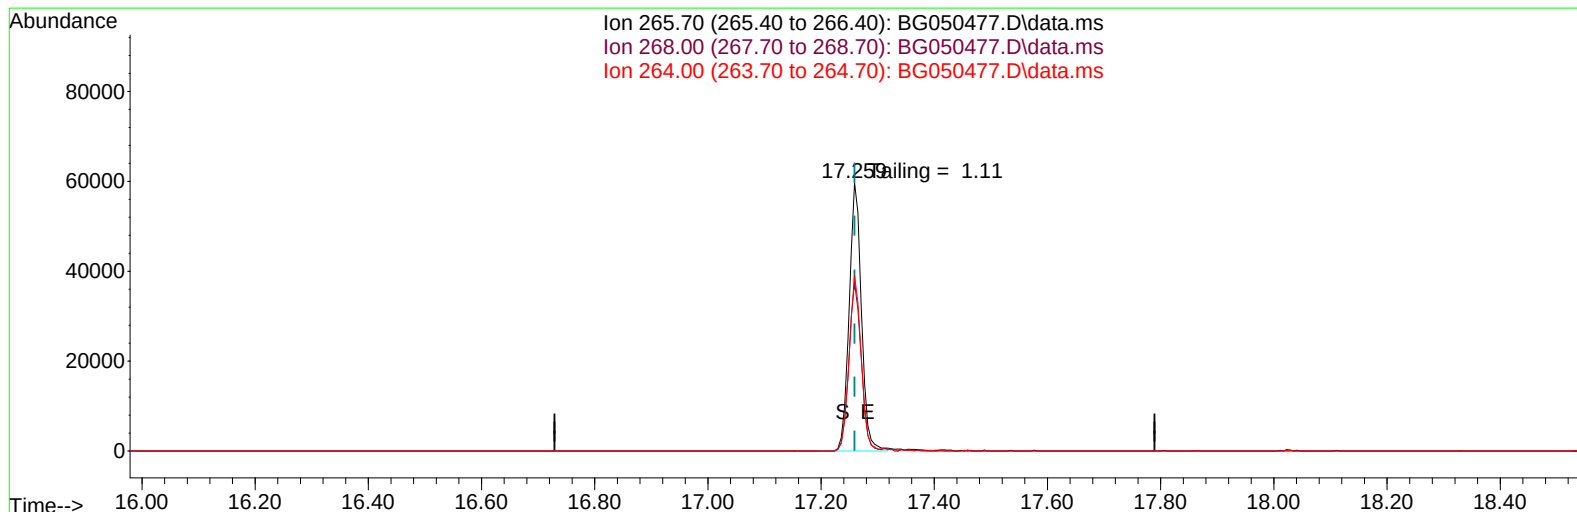

TIC: BG050477.D\data.ms

(70) Pentachlorophenol (C)

17.259min (+ 0.000) 17235.74 ng




response 90718

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	62.66
264.00	61.30	65.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100721\
Data File : BG050477.D
Acq On : 7 Oct 2021 9:51
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 07 13:13:11 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 06 15:51:01 2021
Response via : Initial Calibration

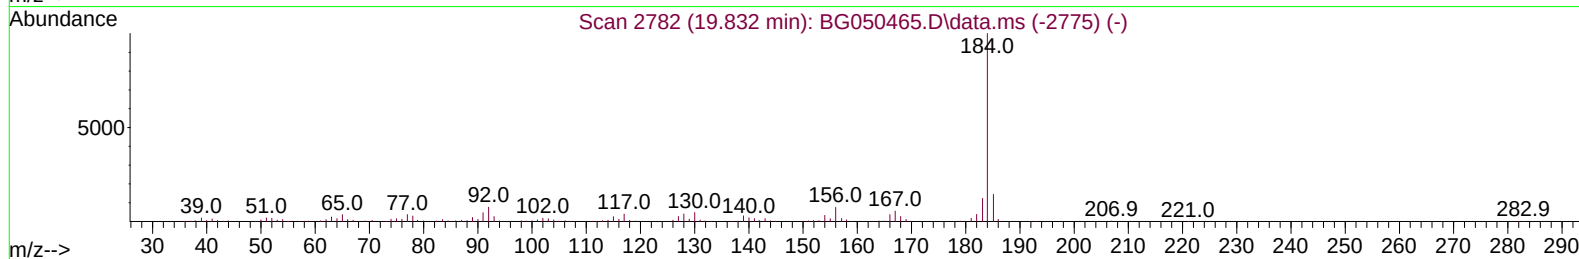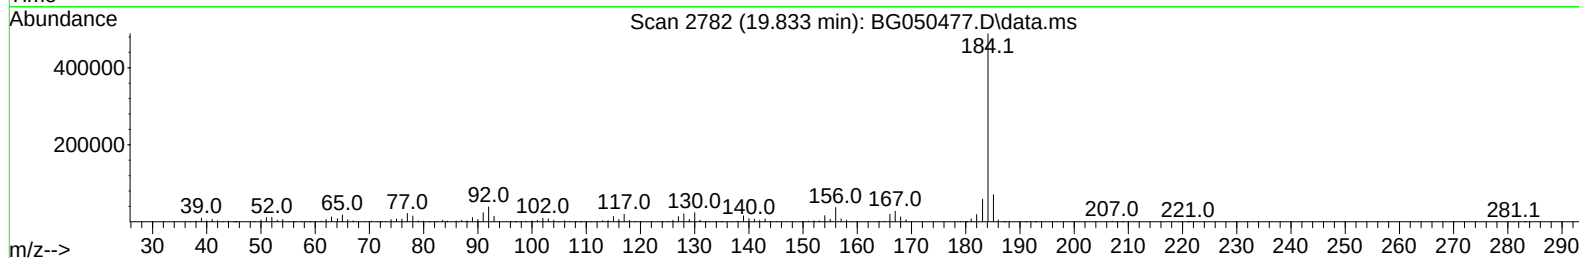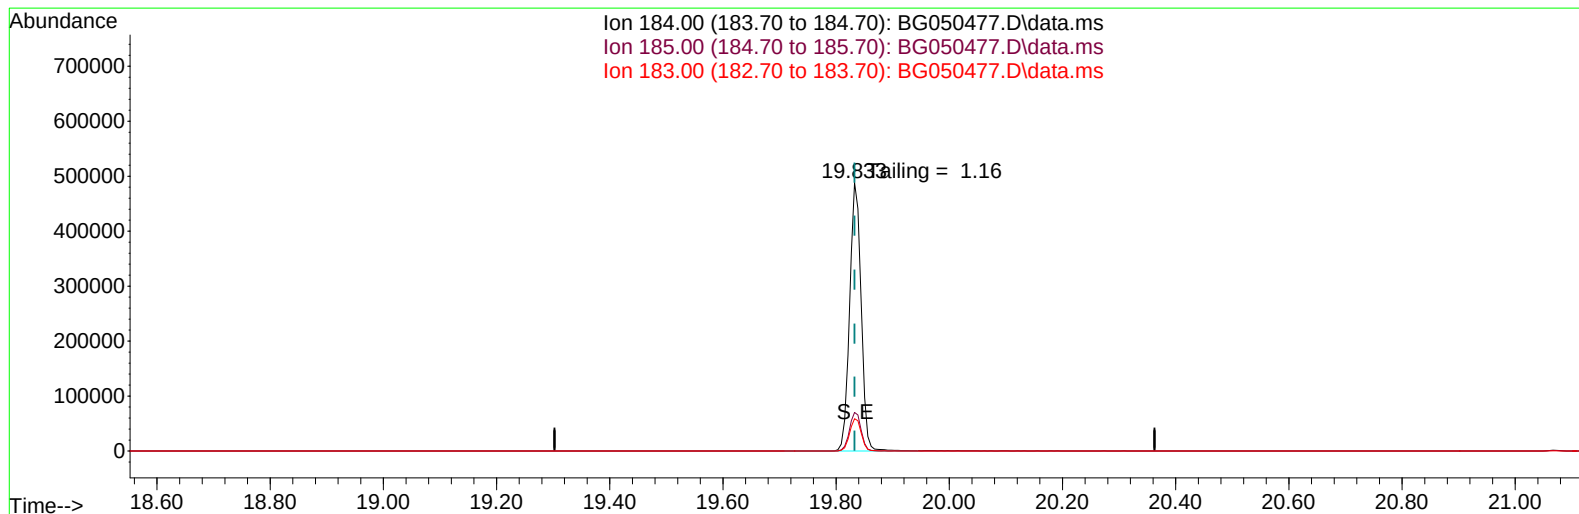

TIC: BG050477.D\data.ms

(77) Benzidine

19.833min (+ 0.000) 0.00 ng

response 690577

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	14.38
183.00	11.70	12.07
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_G
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
10/7/2021	BNA_G	<u>BG050477.D</u>
Compound Name	Response	Retention Time
DDT	292711	21.07
DDD	13456	20.62
DDE	256	20.11
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
13712	306423	4.47