
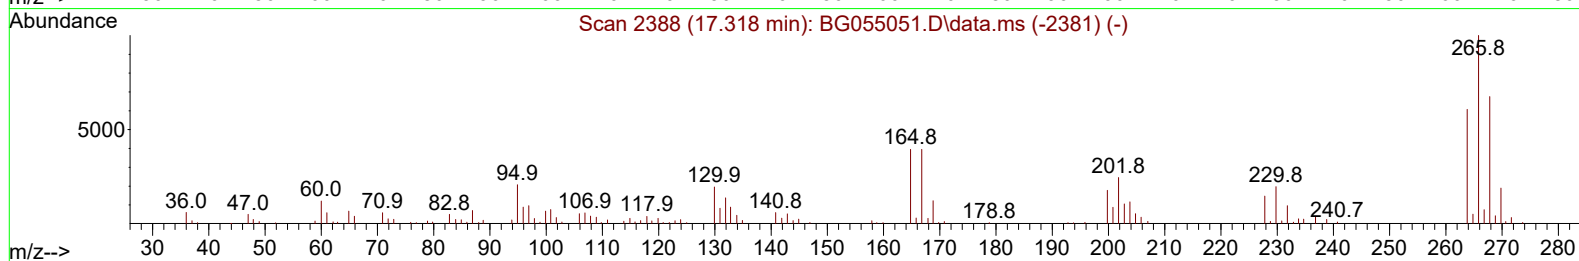
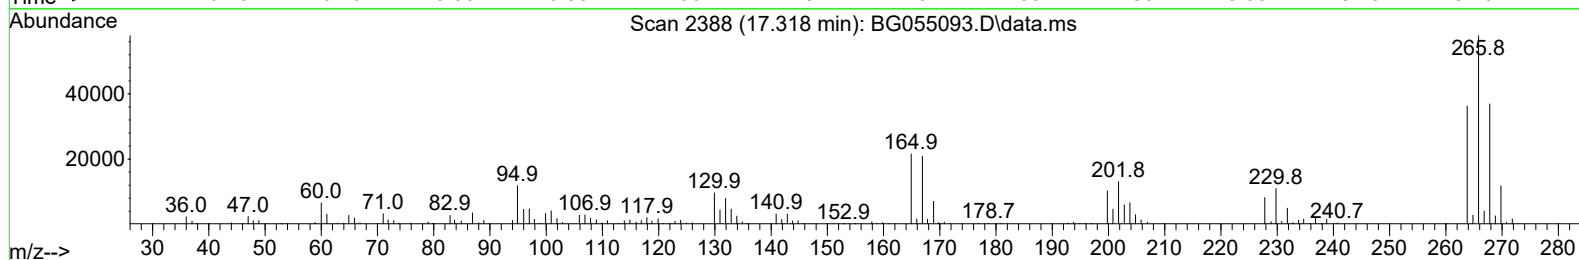


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100722\
Data File : BG055093.D
Acq On : 7 Oct 2022 9:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 08 05:40:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 08 03:04:59 2022
Response via : Initial Calibration

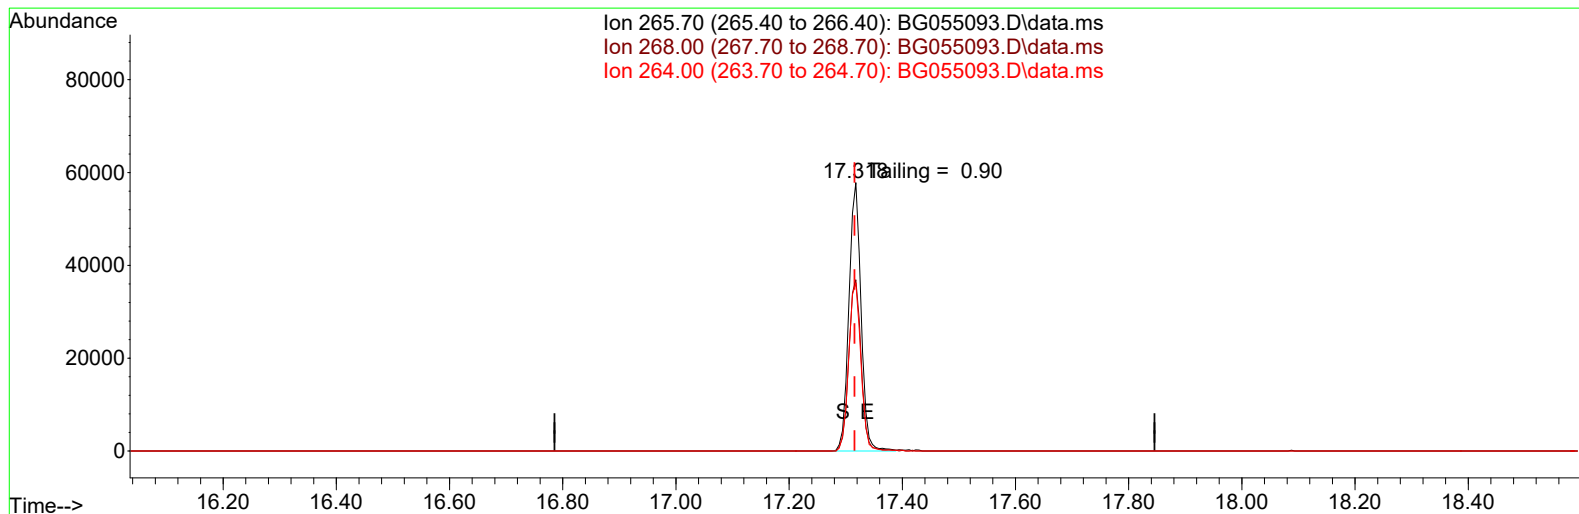

TIC: BG055093.D\data.ms

(70) Pentachlorophenol (C)




17.318min (+ 0.003) 36761.42 ng

response 85934

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.50	63.81
264.00	60.80	62.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100722\
Data File : BG055093.D
Acq On : 7 Oct 2022 9:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 08 05:40:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 08 03:04:59 2022
Response via : Initial Calibration

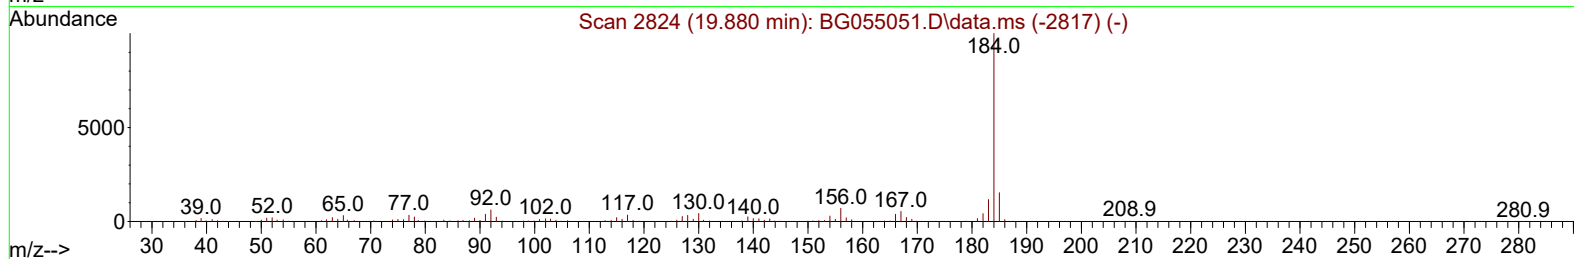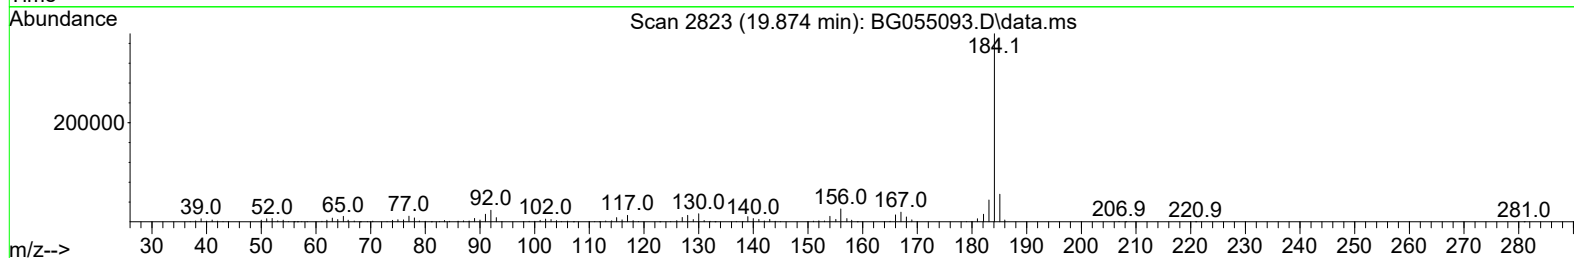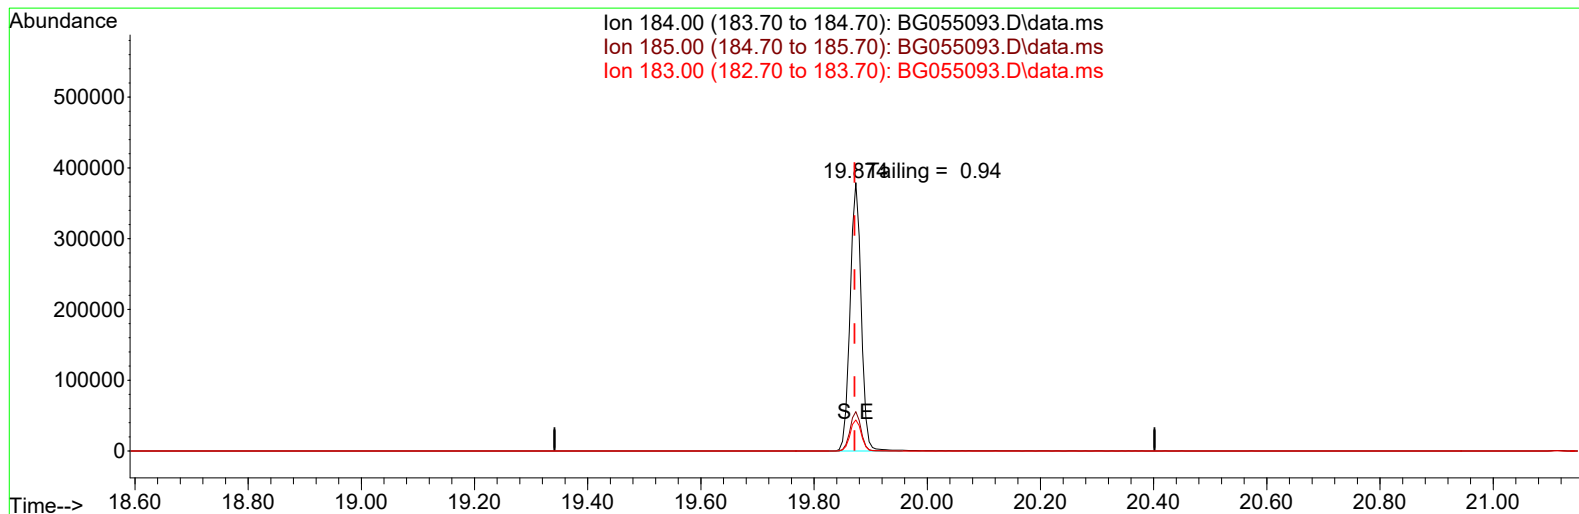

TIC: BG055093.D\data.ms

(77) Benzidine

19.874min (+ 0.003) 0.00 ng



response 517470

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.70
183.00	11.70	11.60
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100722\
 Data File : BG055093.D
 Acq On : 7 Oct 2022 9:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Oct 08 03:04:59 2022

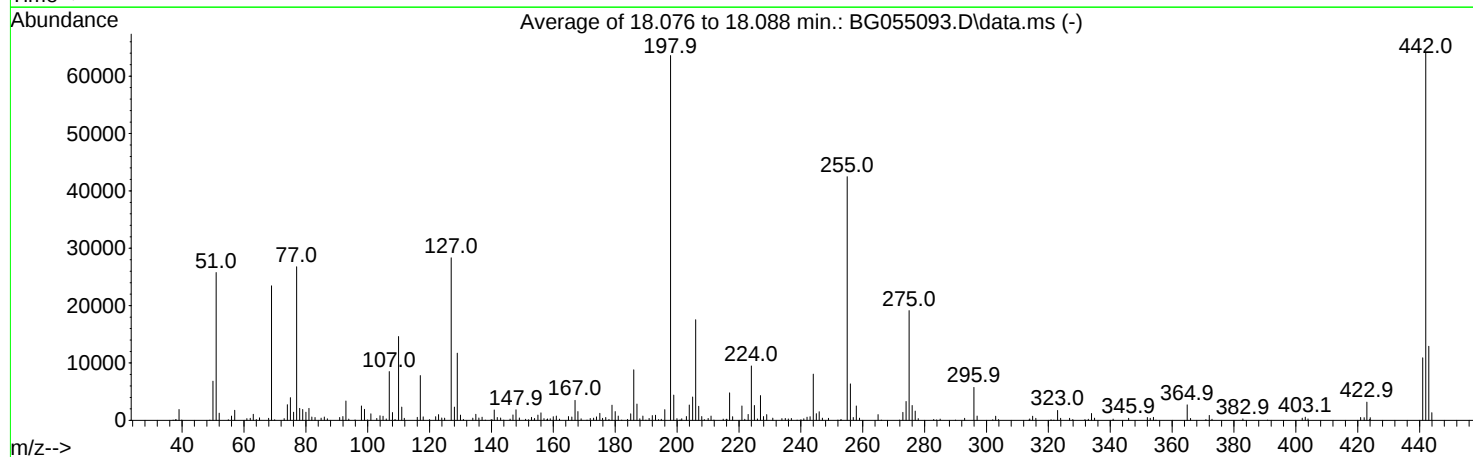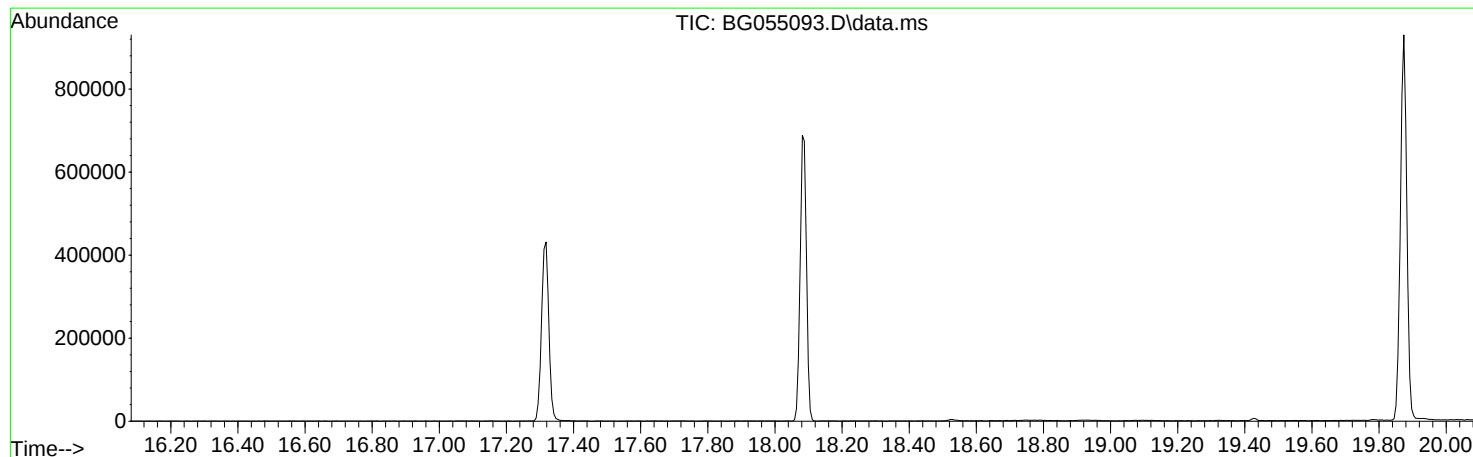

AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2511

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.5	25784	PASS
68	69	0.00	2	1.5	363	PASS
69	198	0.00	100	36.9	23448	PASS
70	69	0.00	2	0.5	118	PASS
127	198	10	80	44.6	28341	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	63600	PASS
199	198	5	9	7.0	4421	PASS
275	198	10	60	30.1	19135	PASS
365	198	1	100	4.2	2702	PASS
441	198	0.01	100	17.1	10904	PASS
442	442	50	100	100.0	64125	PASS
443	442	15	24	20.1	12914	PASS

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/7/2022	BNA_G	<u>BG055093.D</u>
Compound Name	Response	Retention Time
DDT	231234	21.113
DDD	4921	20.655
DDE	0	20.162
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4921	236155	2.08