
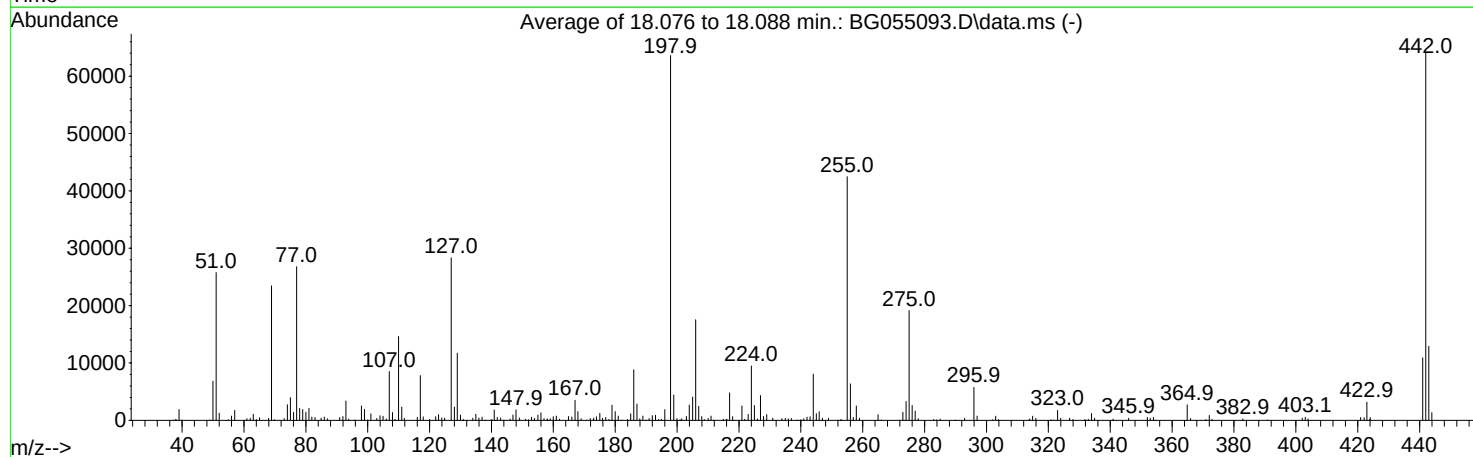


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100722\
 Data File : BG055093.D
 Acq On : 7 Oct 2022 9:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Oct 08 03:04:59 2022

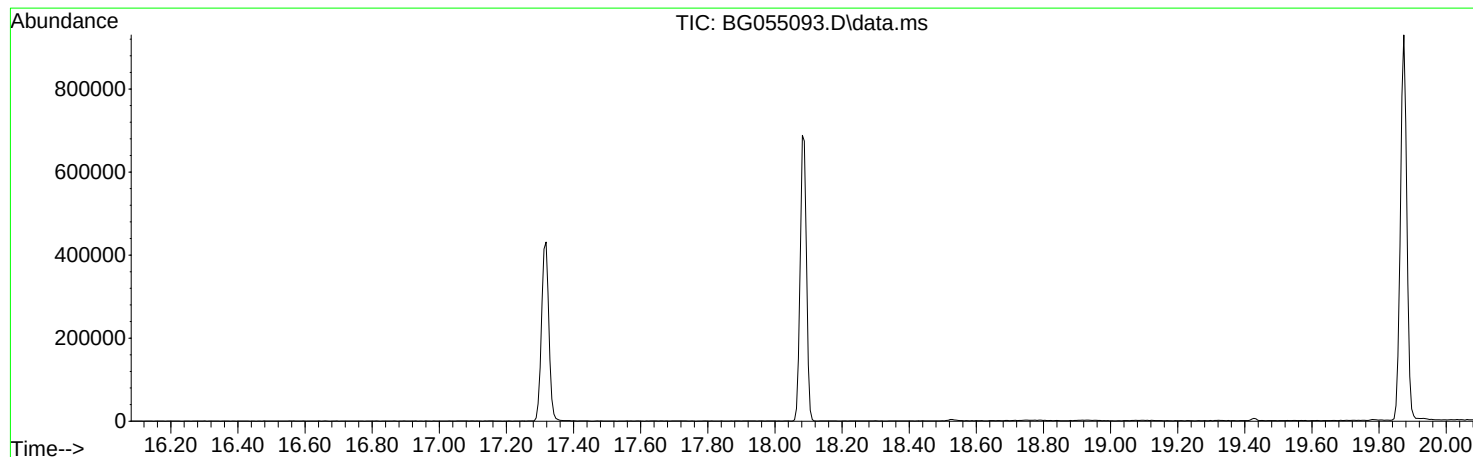




AutoFind: Scans 2517, 2518, 2519; Background Corrected with Scan 2511

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.5	25784	PASS
68	69	0.00	2	1.5	363	PASS
69	198	0.00	100	36.9	23448	PASS
70	69	0.00	2	0.5	118	PASS
127	198	10	80	44.6	28341	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	63600	PASS
199	198	5	9	7.0	4421	PASS
275	198	10	60	30.1	19135	PASS
365	198	1	100	4.2	2702	PASS
441	198	0.01	100	17.1	10904	PASS
442	442	50	100	100.0	64125	PASS
443	442	15	24	20.1	12914	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100722\
Data File : BG055093.D
Acq On : 7 Oct 2022 9:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 08 05:40:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 08 03:04:59 2022
Response via : Initial Calibration

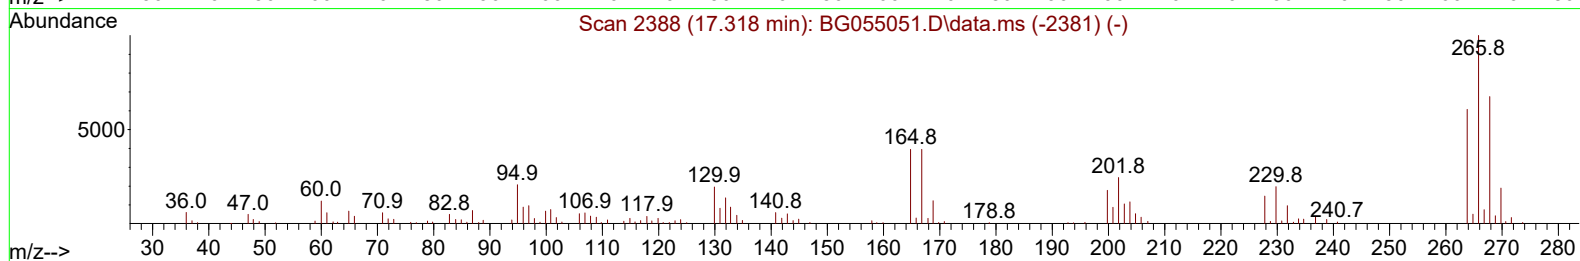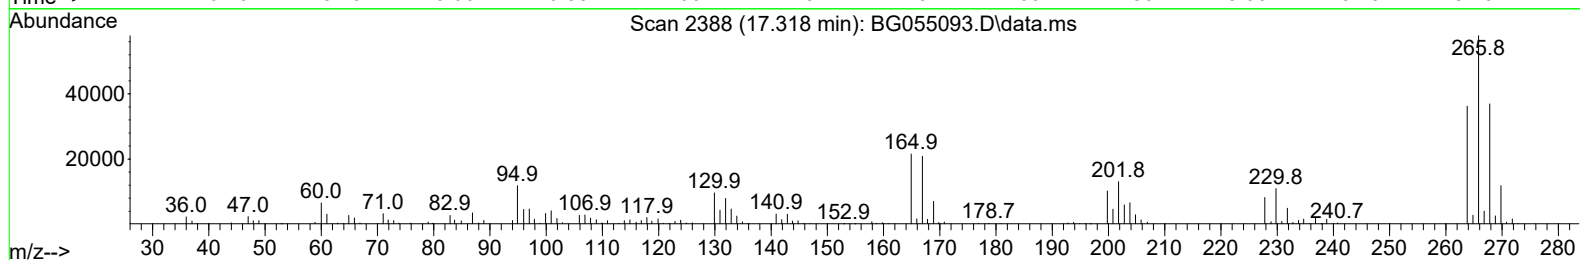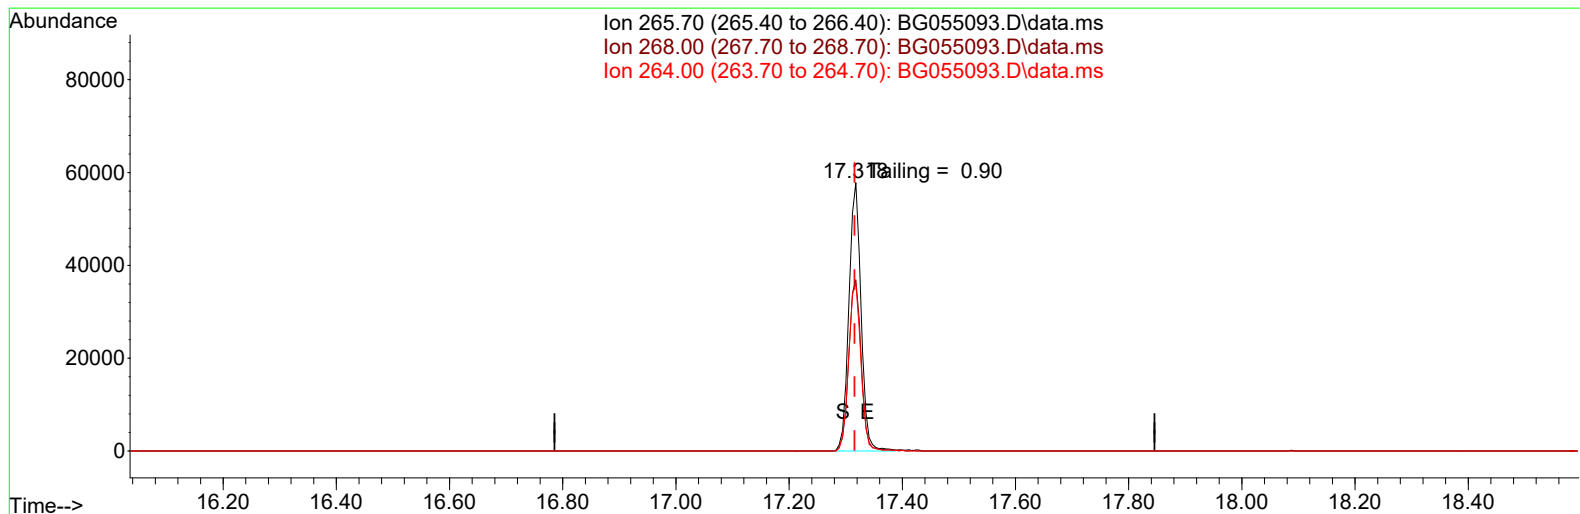

TIC: BG055093.D\data.ms

(70) Pentachlorophenol (C)

17.318min (+ 0.003) 36761.42 ng




response 85934

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.50	63.81
264.00	60.80	62.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100722\
Data File : BG055093.D
Acq On : 7 Oct 2022 9:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 08 05:40:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 08 03:04:59 2022
Response via : Initial Calibration

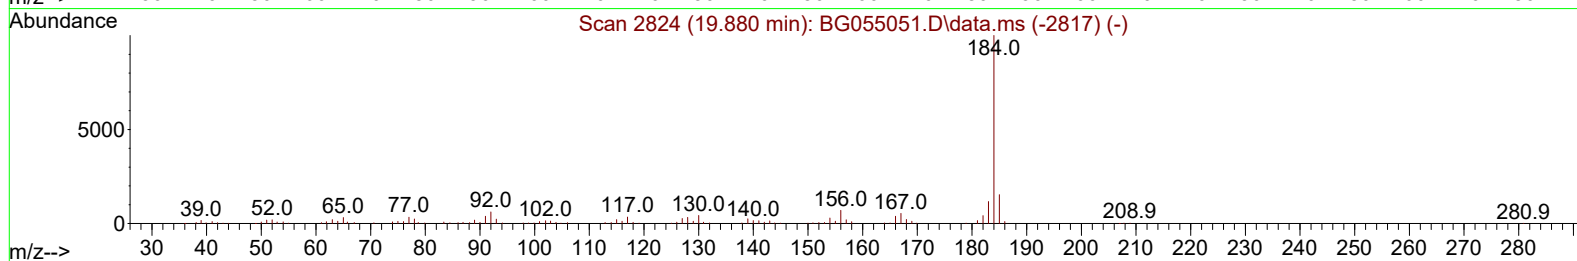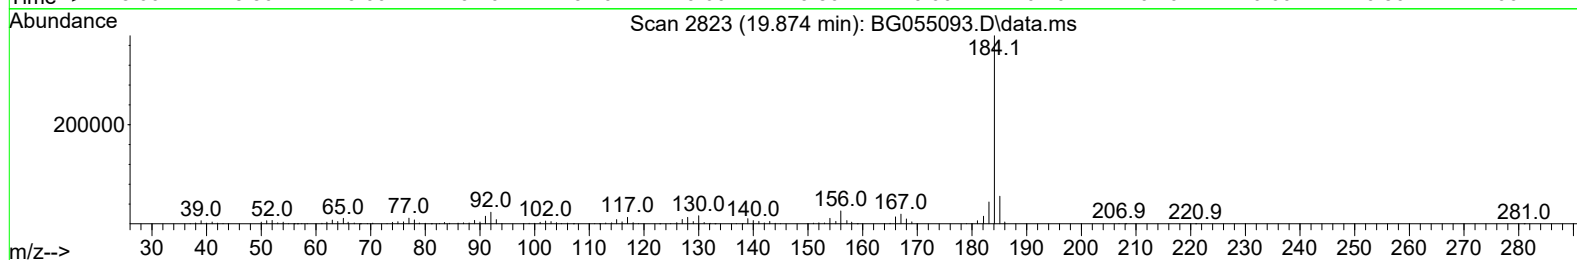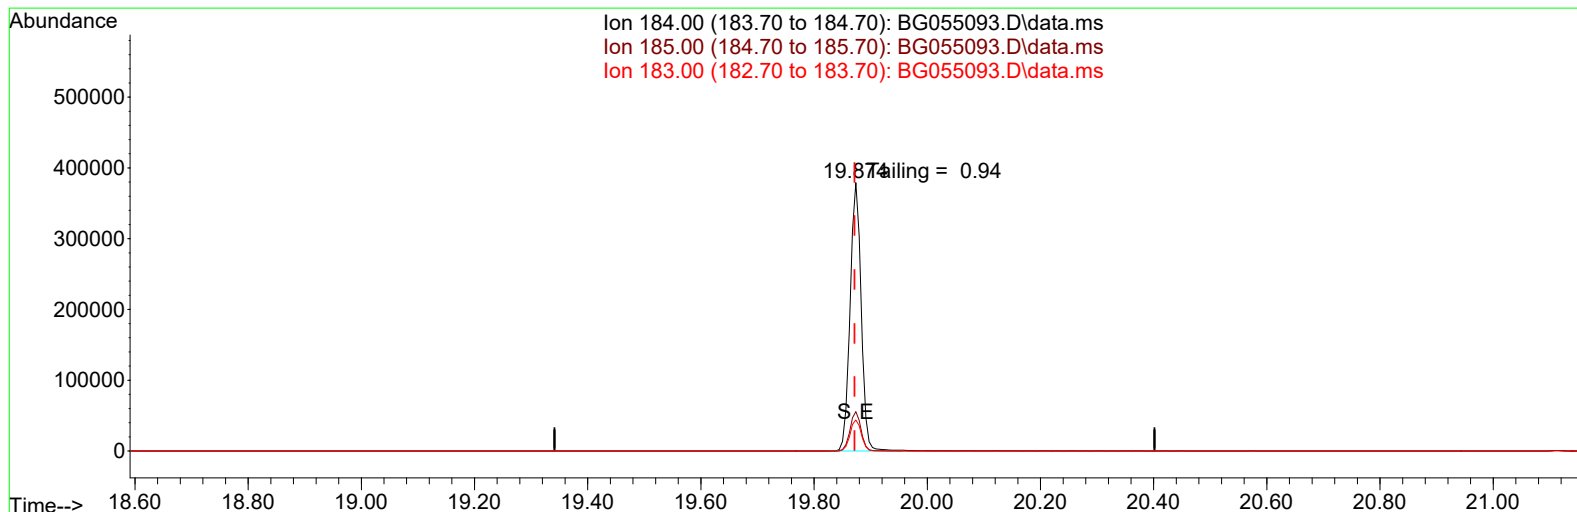

TIC: BG055093.D\data.ms

(77) Benzidine

19.874min (+ 0.003) 0.00 ng

response 517470

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	14.70
183.00	11.70	11.60
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/7/2022	BNA_G	<u>BG055093.D</u>
Compound Name	Response	Retention Time
DDT	231234	21.113
DDD	4921	20.655
DDE	0	20.162
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4921	236155	2.08

Instrument :
BNA_G
ClientSampleId :
DFTPP