
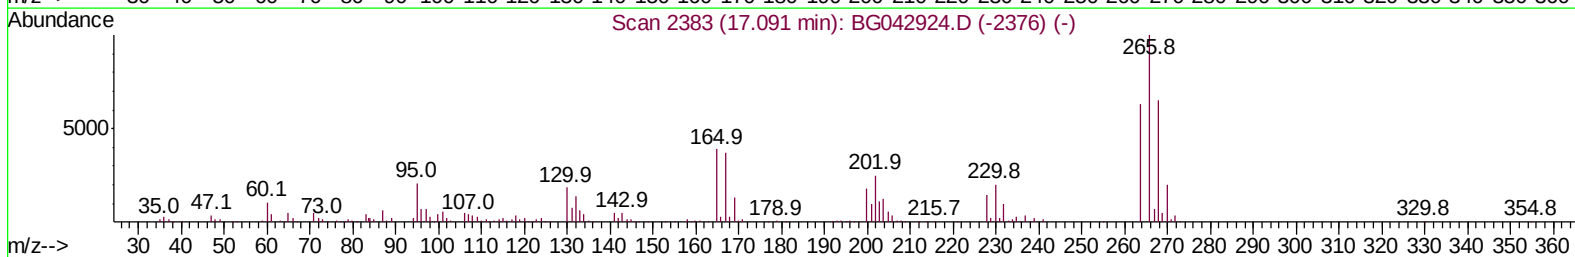
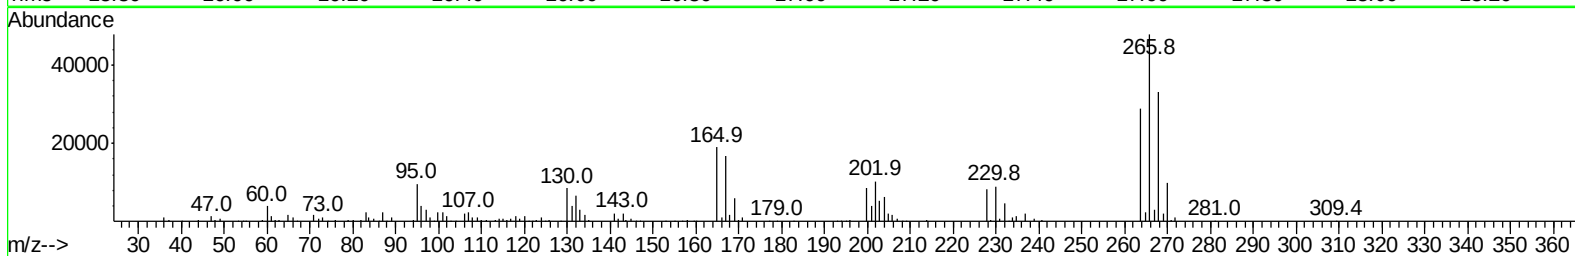


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG100819\
Data File : BG043082.D
Acq On : 8 Oct 2019 10:44
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 09 02:40:19 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 09 01:11:45 2019
Response via : Initial Calibration

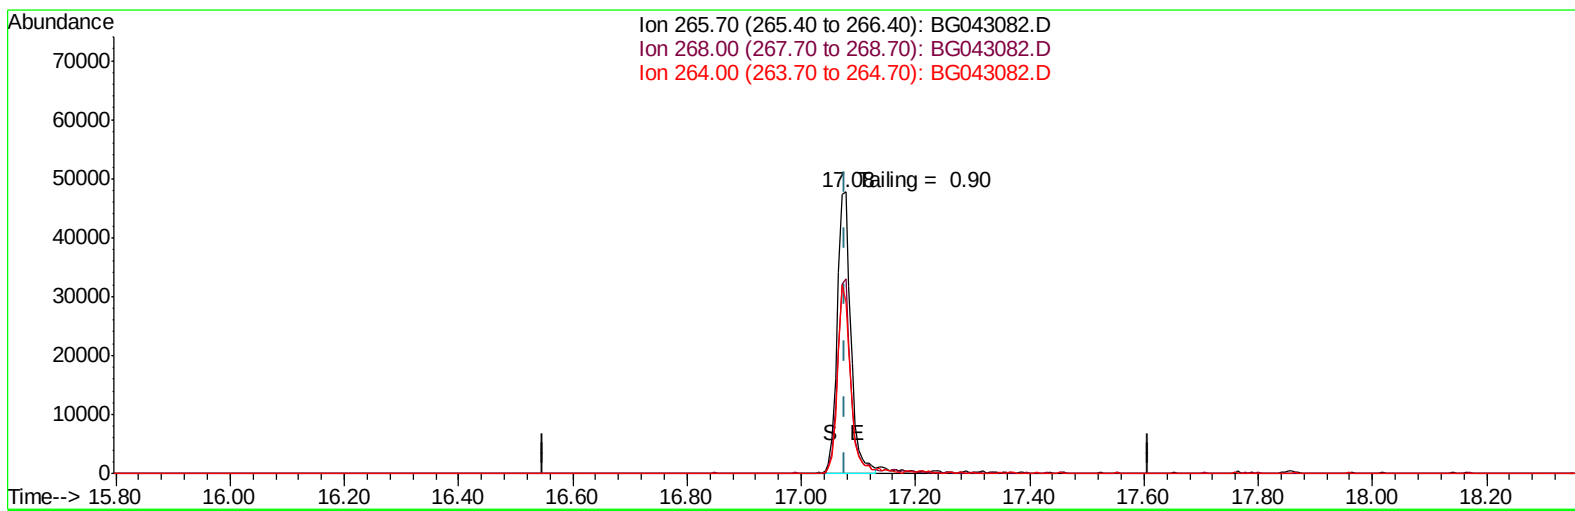

TIC: BG043082.D

(70) Pentachlorophenol (C)




17.077min (-0.001) 26653.23ng

response 78877

Ion	Exp%	Act%
265.70	100	100
268.00	65.20	69.15
264.00	63.40	60.74
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG100819\
 Data File : BG043082.D
 Acq On : 8 Oct 2019 10:44
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 09 02:40:19 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA G\METHODS\8270-BG092519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 09 01:11:45 2019
 Response via : Initial Calibration

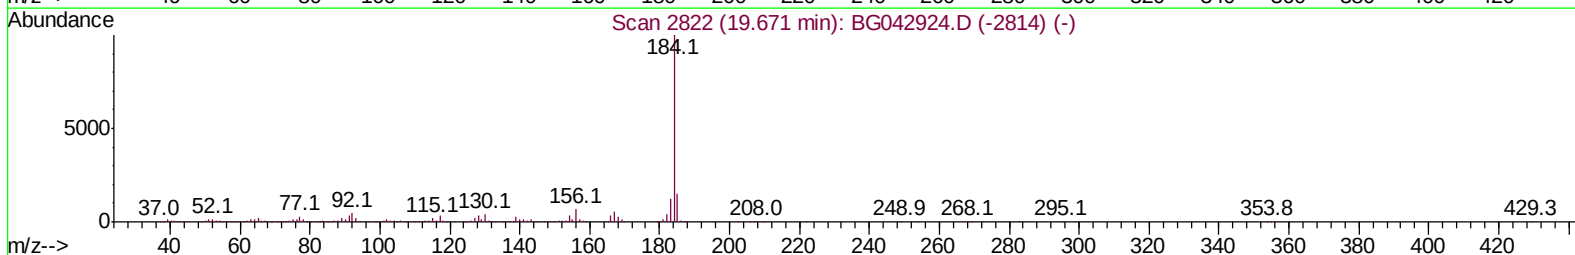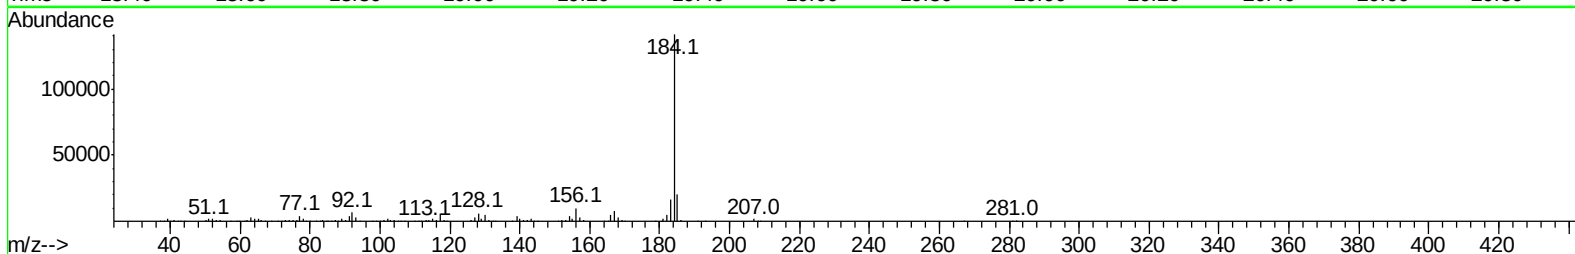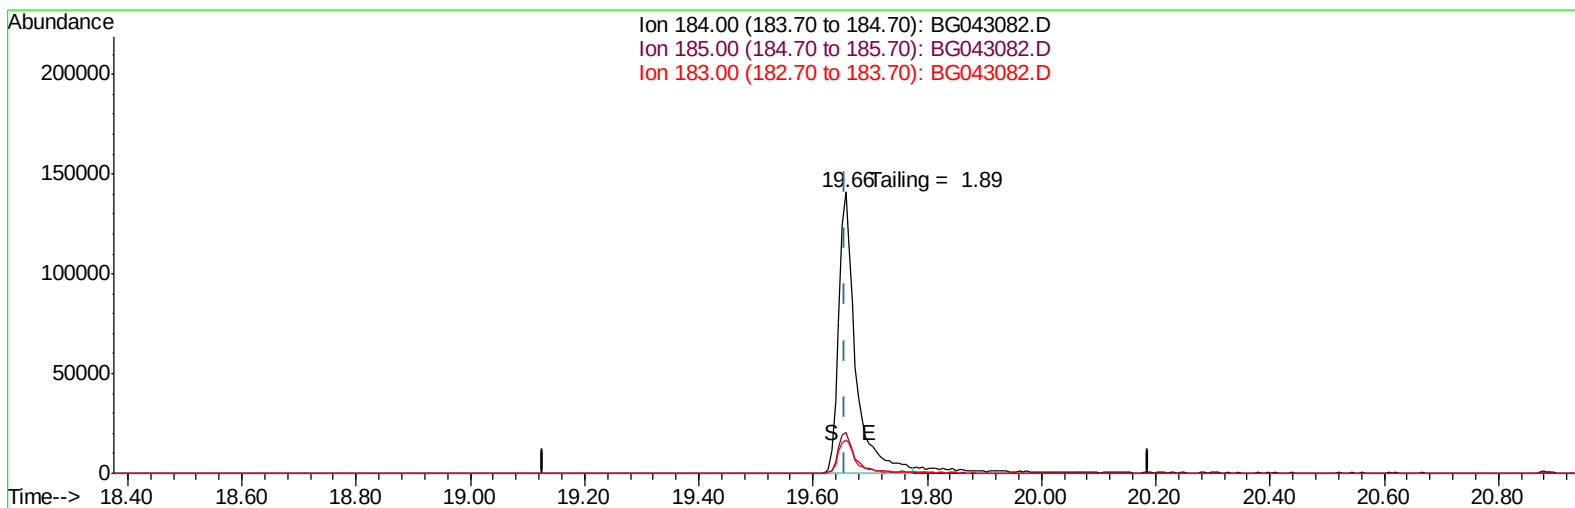

TIC: BG043082.D

(77) Benzidine

19.656min (-0.001) 134671.83ng

response 293368

Ion	Exp%	Act%
184.00	100	100
185.00	14.80	14.39
183.00	12.60	12.00
0.00	0.00	0.00