


Data Path : Z:\SVOASRV\HPCHEM1\BNA G\DATA\BG100819\
 Data File : BG043082.D
 Acq On : 8 Oct 2019 10:44
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 09 01:11:45 2019

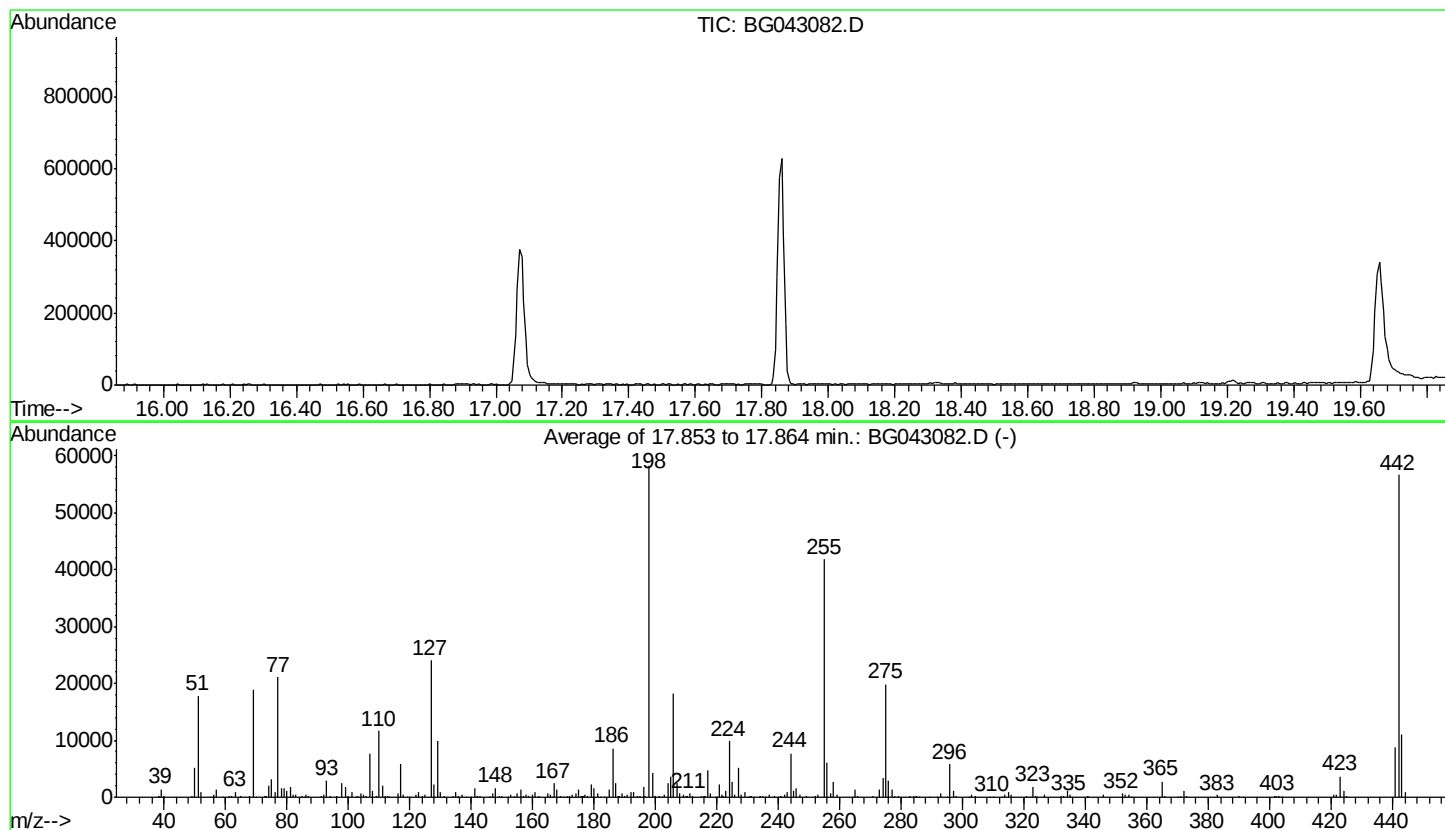

AutoFind: Scans 2513, 2514, 2515; Background Corrected with Scan 2506

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.5	17808	PASS
68	69	0.00	2	0.9	177	PASS
69	198	0.00	100	32.3	18835	PASS
70	69	0.00	2	0.4	73	PASS
127	198	10	80	41.3	24080	PASS
197	198	0.00	2	0.3	199	PASS
198	198	100	100	100.0	58301	PASS
199	198	5	9	7.3	4283	PASS
275	198	10	60	34.1	19885	PASS
365	198	1	100	4.8	2788	PASS
441	198	0.01	100	15.0	8731	PASS
442	198	50	100	97.1	56626	PASS
443	442	15	24	19.5	11015	PASS