
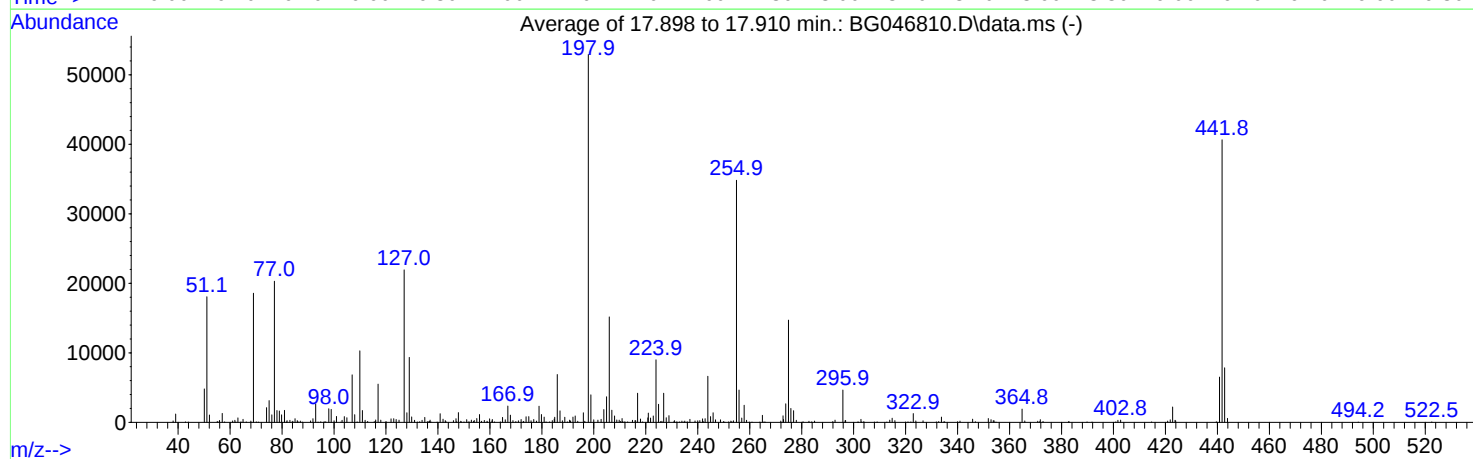


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100820\
Data File : BG046810.D
Acq On : 8 Oct 2020 10:23
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG092220.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 07 11:38:17 2020

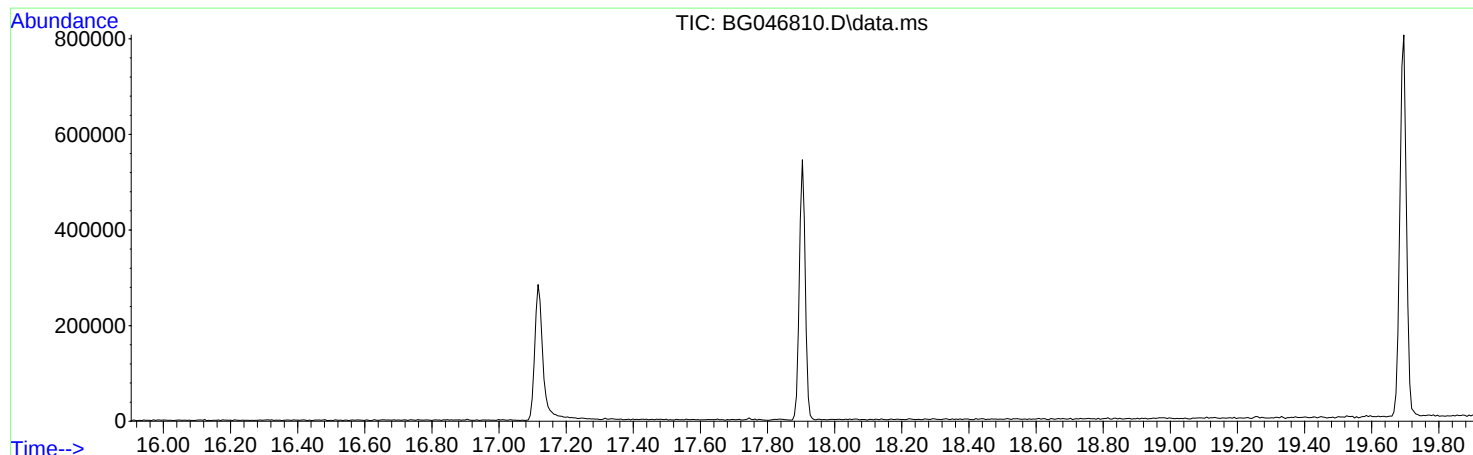

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.2	18080	PASS
68	69	0.00	2	1.0	186	PASS
69	198	0.00	100	35.1	18586	PASS
70	69	0.00	2	0.3	61	PASS
127	198	10	80	41.5	21941	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	52920	PASS
199	198	5	9	7.5	3966	PASS
275	198	10	60	27.8	14705	PASS
365	198	1	100	3.6	1900	PASS
441	198	0.01	100	12.3	6520	PASS
442	198	50	100	76.8	40656	PASS
443	442	15	24	19.3	7850	PASS