
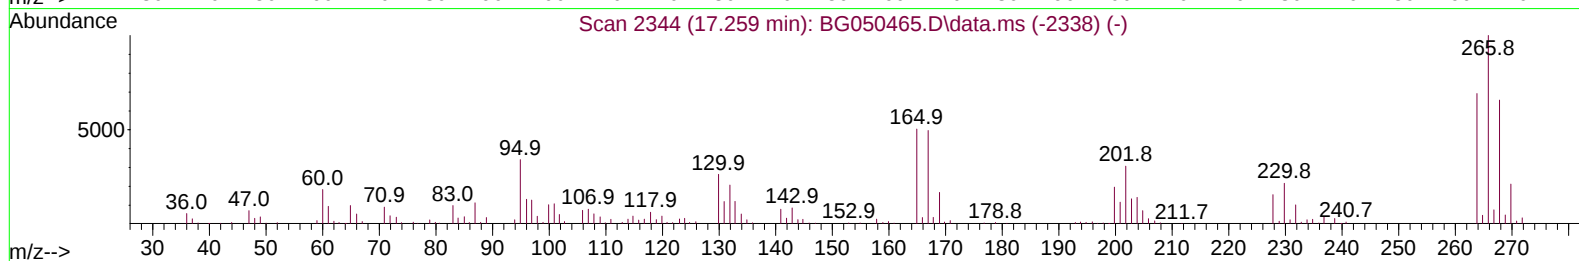
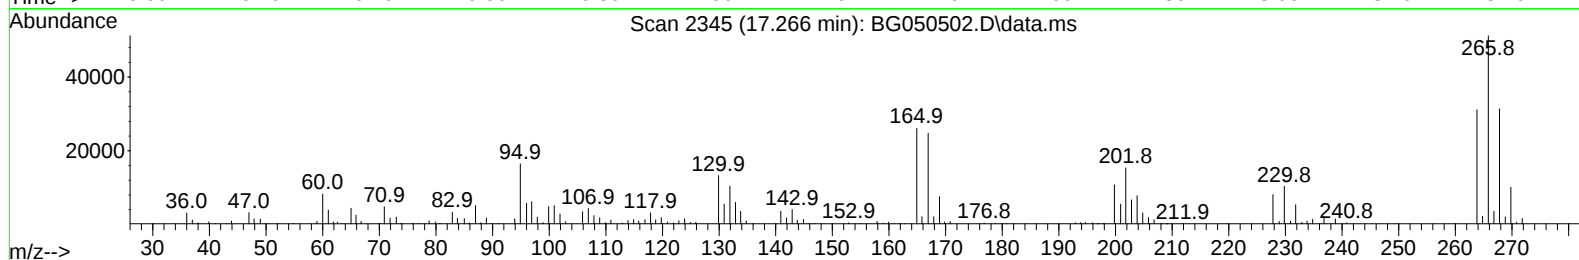


Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG100821\  
Data File : BG050502.D  
Acq On : 8 Oct 2021 8:59  
Operator : CG/JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 08 13:21:39 2021  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG100621.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Oct 06 15:51:01 2021  
Response via : Initial Calibration

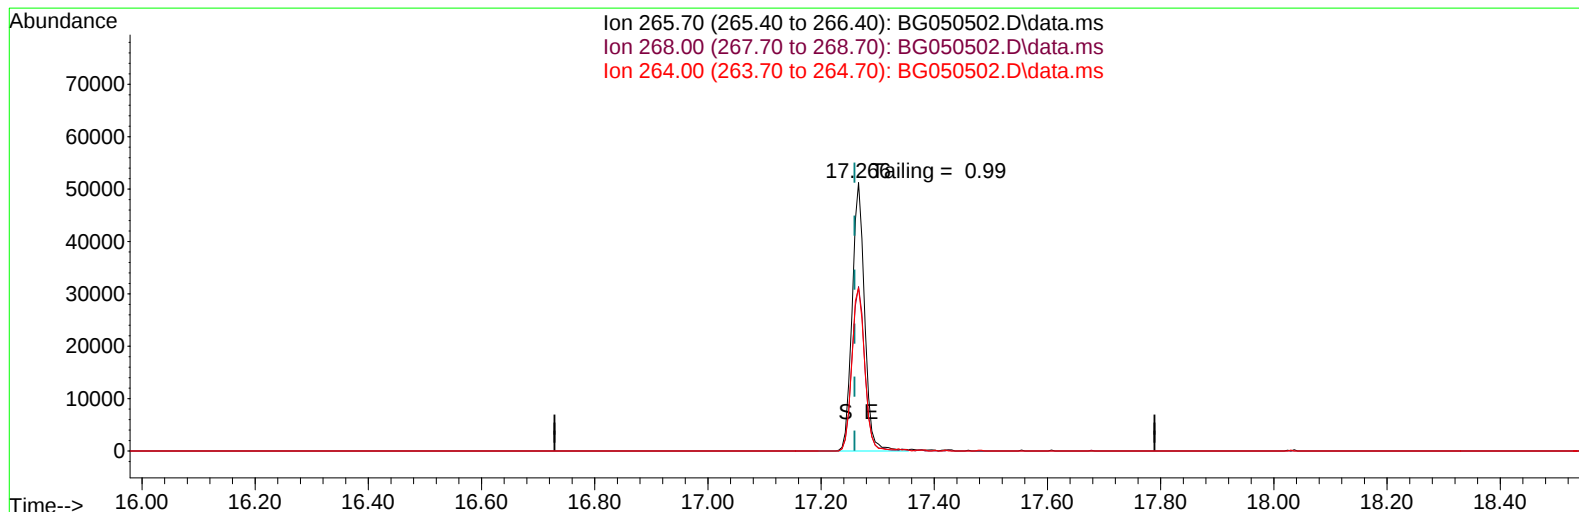

TIC: BG050502.D\data.ms

**(70) Pentachlorophenol (C)**




**17.266min (+ 0.007) 22733.34 ng**

**response 78581**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 61.20  | 61.23  |
| 264.00 | 61.30  | 60.74  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_G\Data\BG100821\  
 Data File : BG050502.D  
 Acq On : 8 Oct 2021 8:59  
 Operator : CG/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 08 13:21:39 2021  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_G\Methods\8270-BG100621.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Oct 06 15:51:01 2021  
 Response via : Initial Calibration

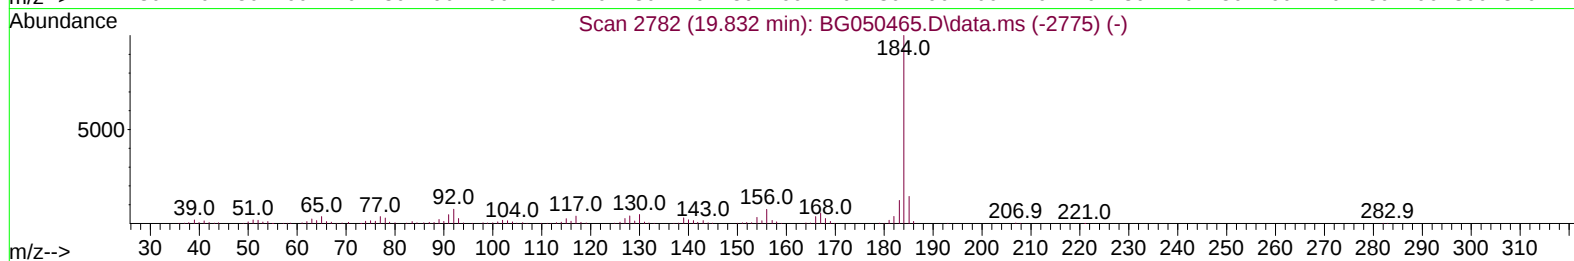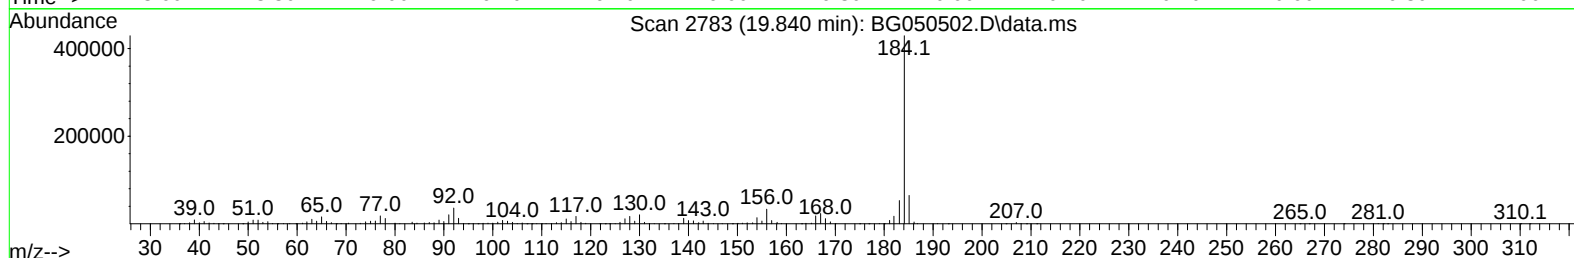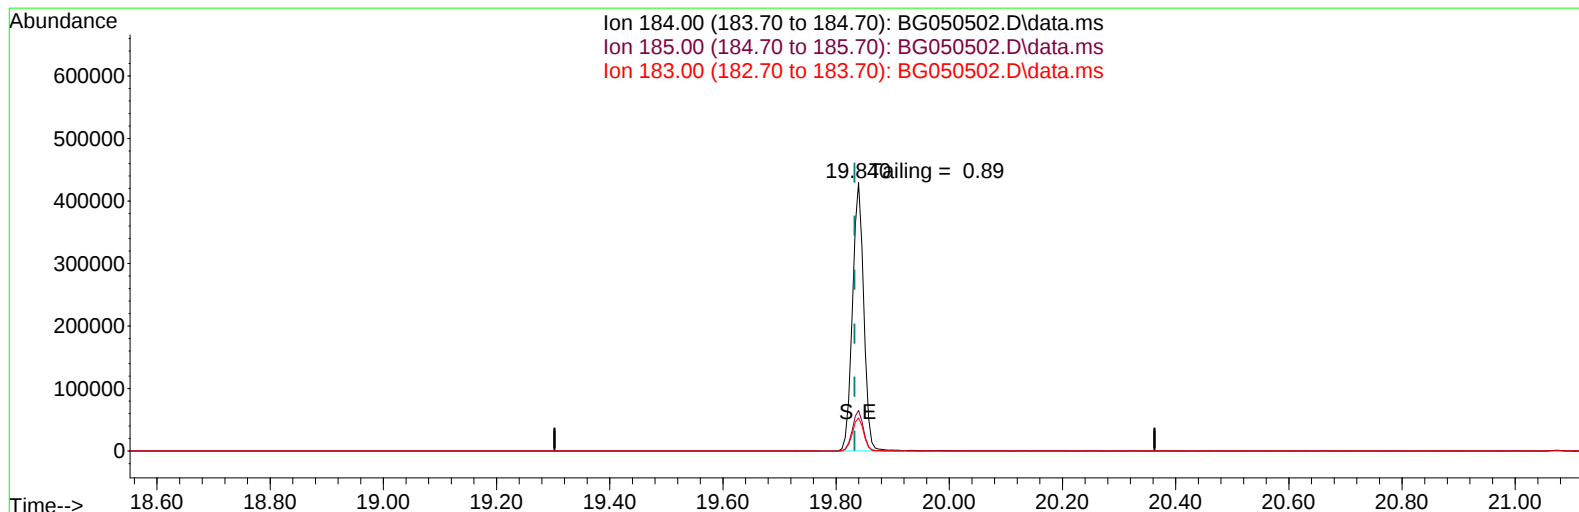

TIC: BG050502.D\data.ms

**(77) Benzidine****19.840min (+ 0.007) 306174.72 ng****response 595409**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.40  | 15.14  |
| 183.00 | 11.70  | 12.37  |
| 0.00   | 0.00   | 0.00   |