


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100821\
 Data File : BG050502.D
 Acq On : 8 Oct 2021 8:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 06 15:51:01 2021

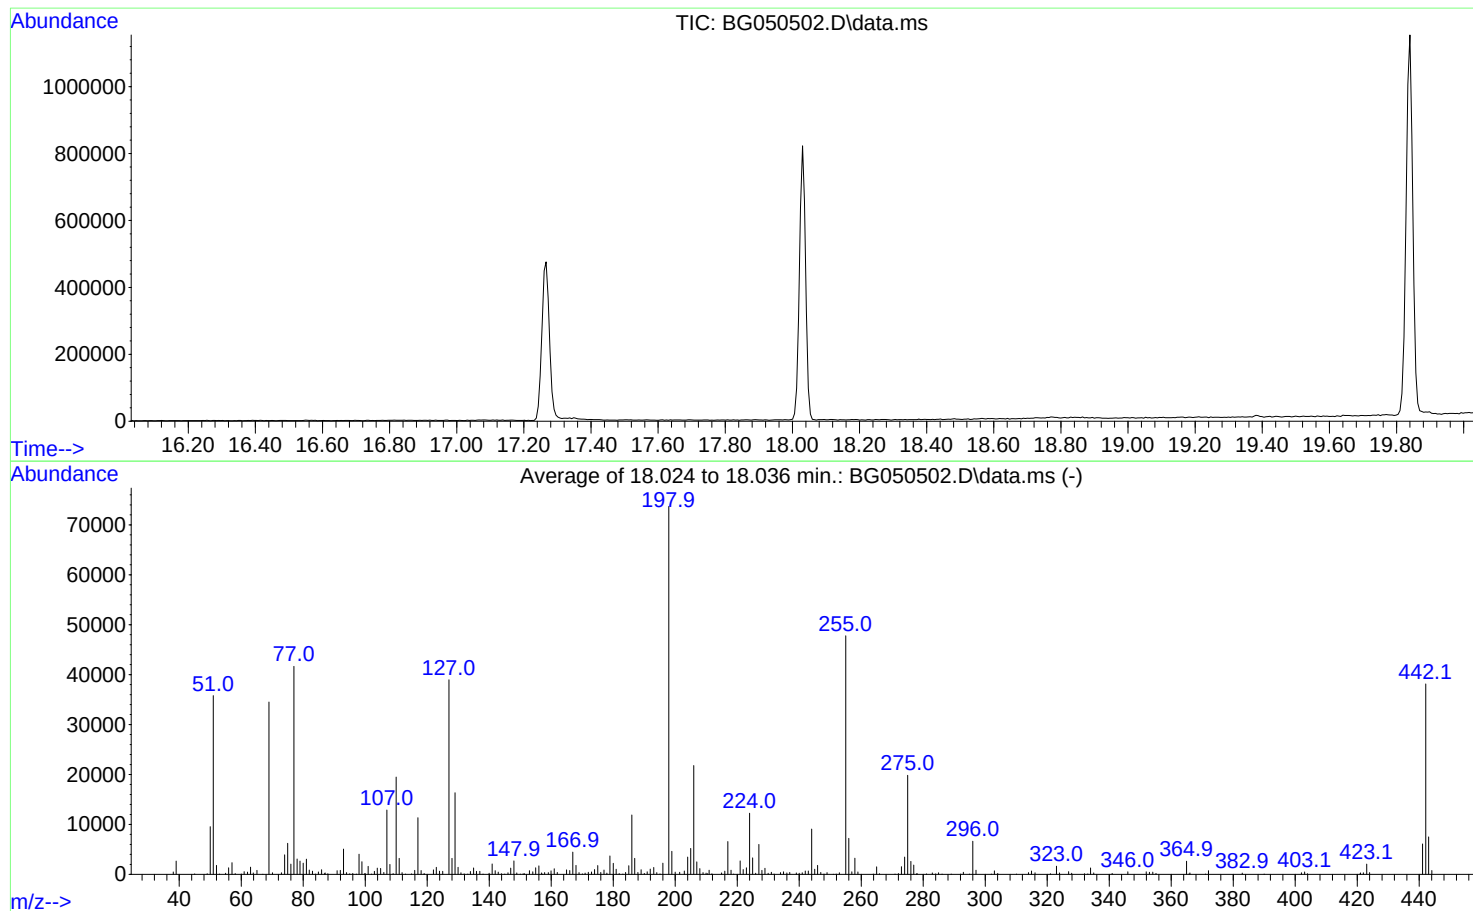




AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2467

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.6	35795	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	46.9	34523	PASS
70	69	0.00	2	0.9	310	PASS
127	198	10	80	52.9	38963	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	73677	PASS
199	198	5	9	6.3	4629	PASS
275	198	10	60	26.9	19829	PASS
365	198	1	100	3.6	2642	PASS
441	198	0.01	100	8.3	6105	PASS
442	442	50	100	100.0	38152	PASS
443	442	15	24	19.7	7506	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100821\
 Data File : BG050502.D
 Acq On : 8 Oct 2021 8:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Oct 08 13:21:39 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 06 15:51:01 2021
 Response via : Initial Calibration

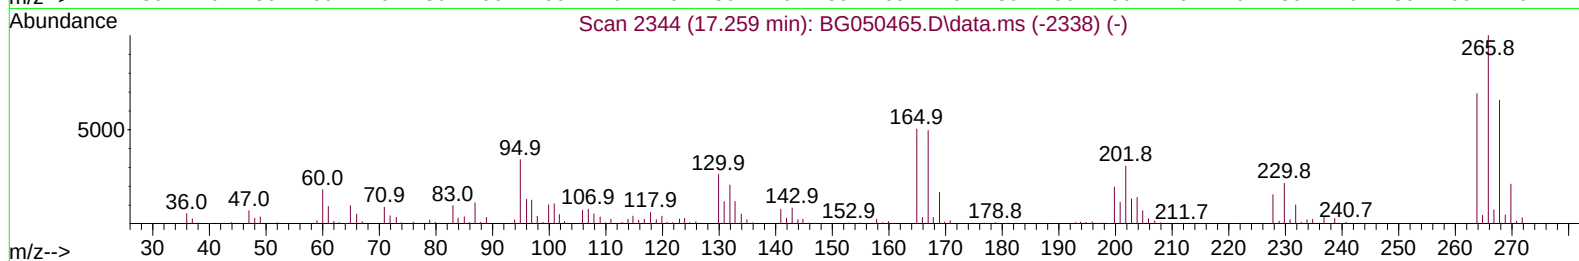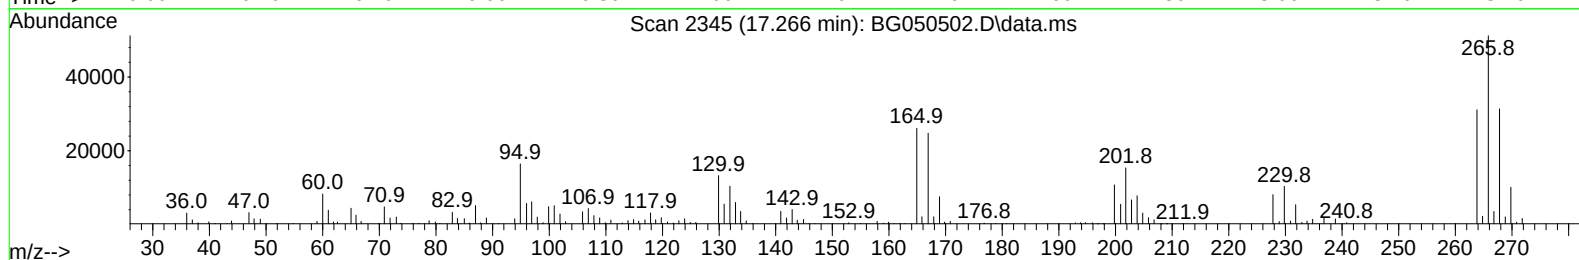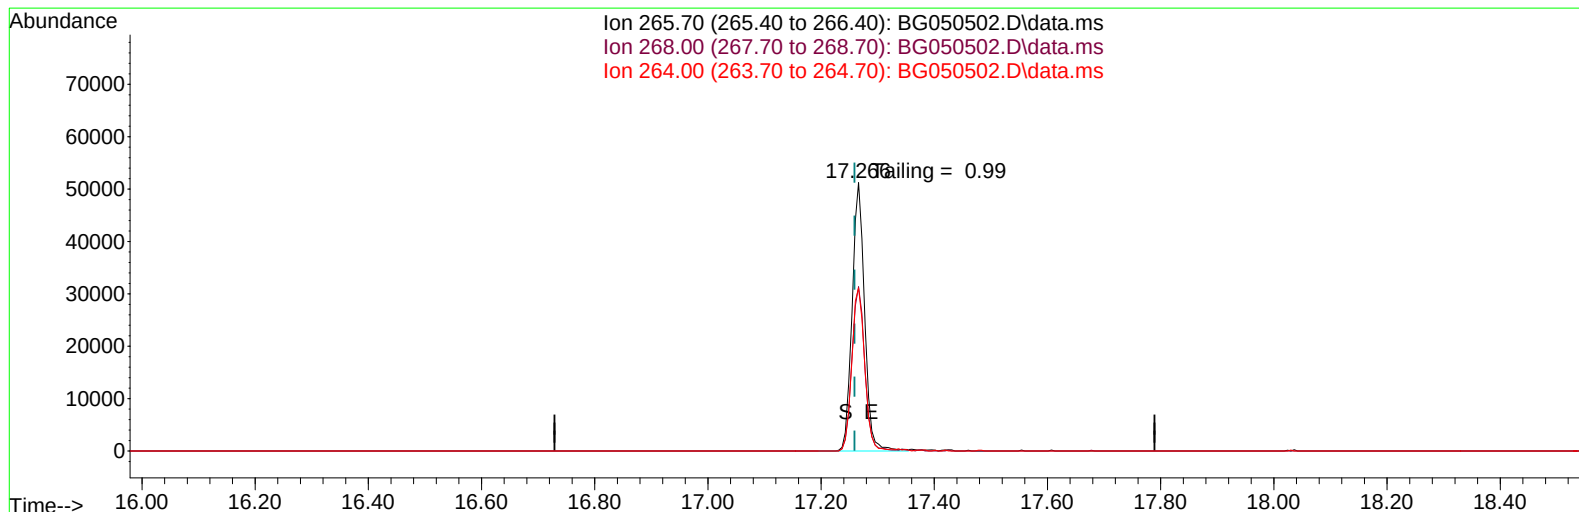

TIC: BG050502.D\data.ms

(70) Pentachlorophenol (C)

17.266min (+ 0.007) 22733.34 ng




response 78581

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	61.23
264.00	61.30	60.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100821\
 Data File : BG050502.D
 Acq On : 8 Oct 2021 8:59
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Oct 08 13:21:39 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 06 15:51:01 2021
 Response via : Initial Calibration

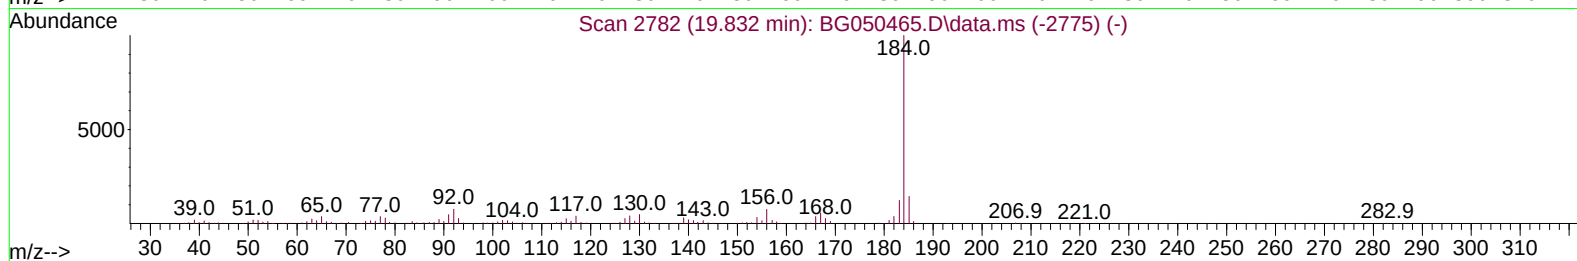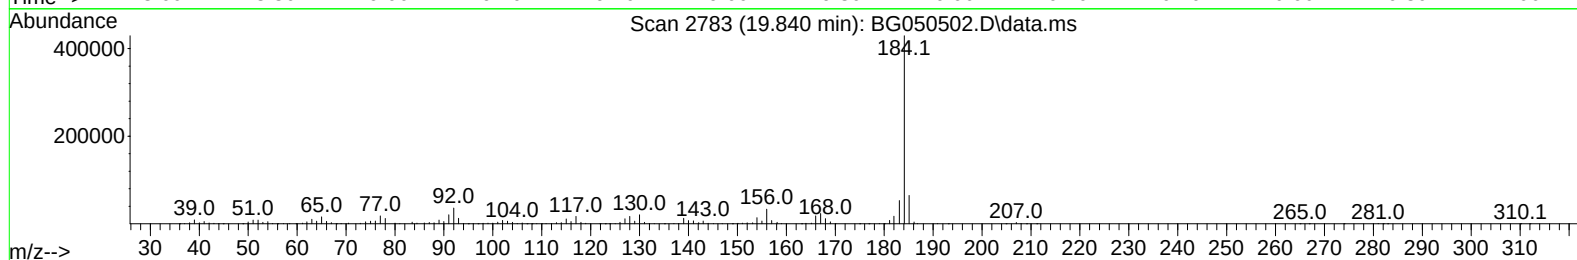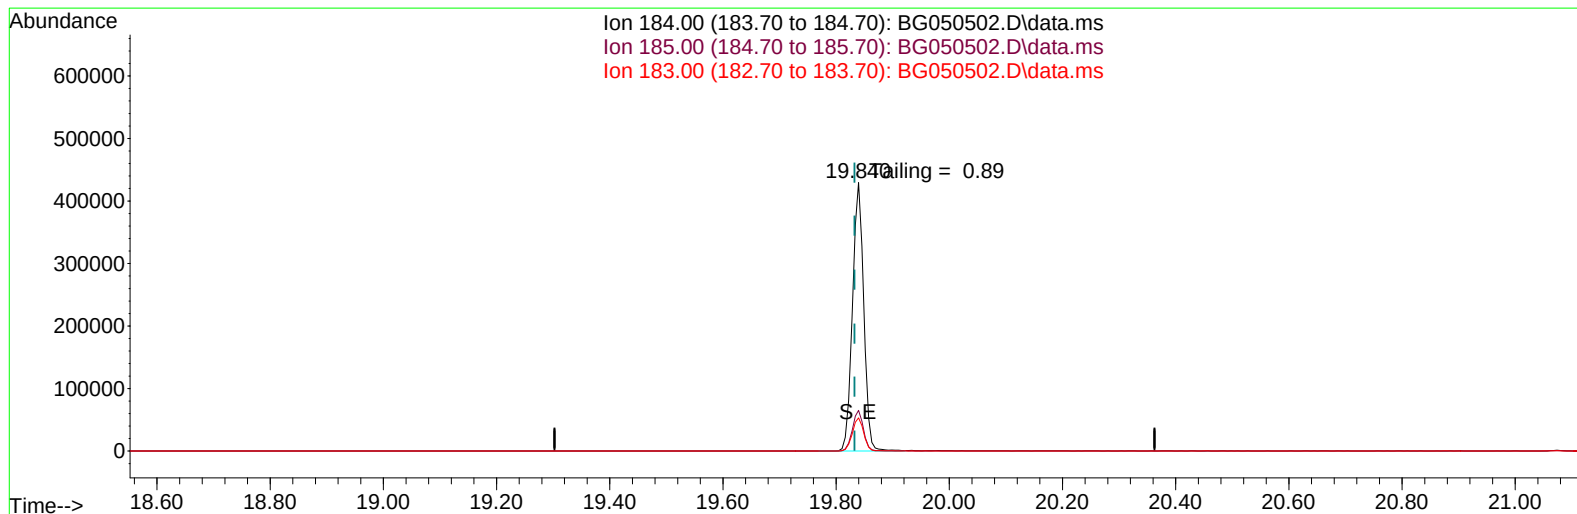

TIC: BG050502.D\data.ms

(77) Benzidine**19.840min (+ 0.007) 306174.72 ng****response 595409**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	15.14
183.00	11.70	12.37
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_G
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
10/8/2021	BNA_G	BG050502.D
Compound Name	Response	Retention Time
DDT	228996	21.07
DDD	10648	20.62
DDE	67	20.07
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10715	239711	4.47