


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100821\
 Data File : BG050512.D
 Acq On : 8 Oct 2021 16:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Oct 06 15:51:01 2021

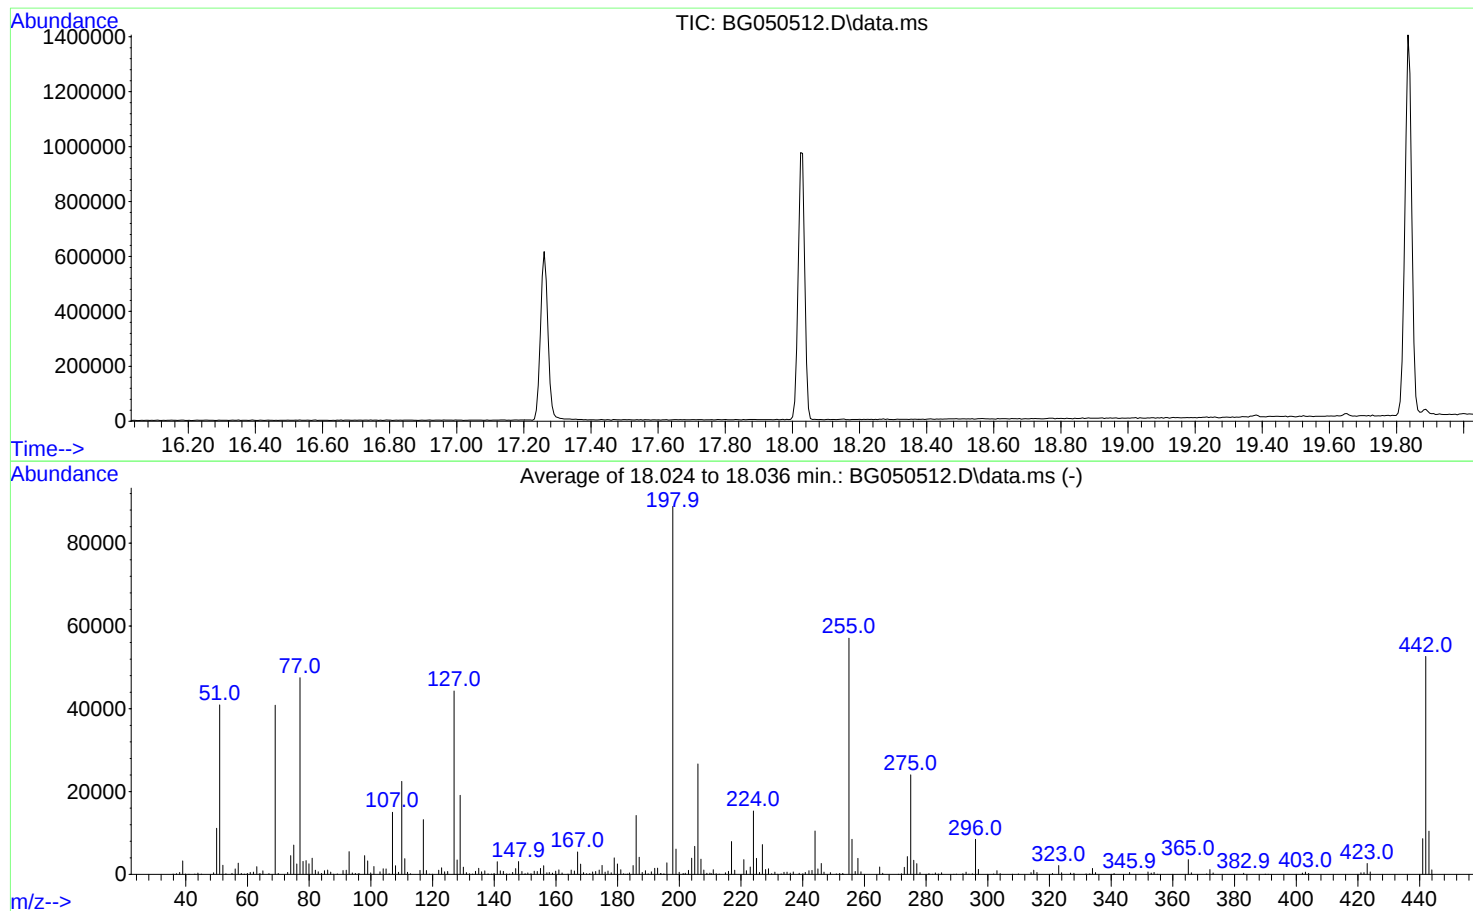




AutoFind: Scans 2474, 2475, 2476; Background Corrected with Scan 2466

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.1	40933	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	46.0	40874	PASS
70	69	0.00	2	0.6	242	PASS
127	198	10	80	49.9	44299	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	88861	PASS
199	198	5	9	6.9	6119	PASS
275	198	10	60	27.0	24024	PASS
365	198	1	100	4.0	3552	PASS
441	198	0.01	100	9.7	8614	PASS
442	442	50	100	100.0	52640	PASS
443	442	15	24	19.9	10454	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100821\
 Data File : BG050512.D
 Acq On : 8 Oct 2021 16:50
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Oct 09 04:58:18 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Oct 06 15:51:01 2021
 Response via : Initial Calibration

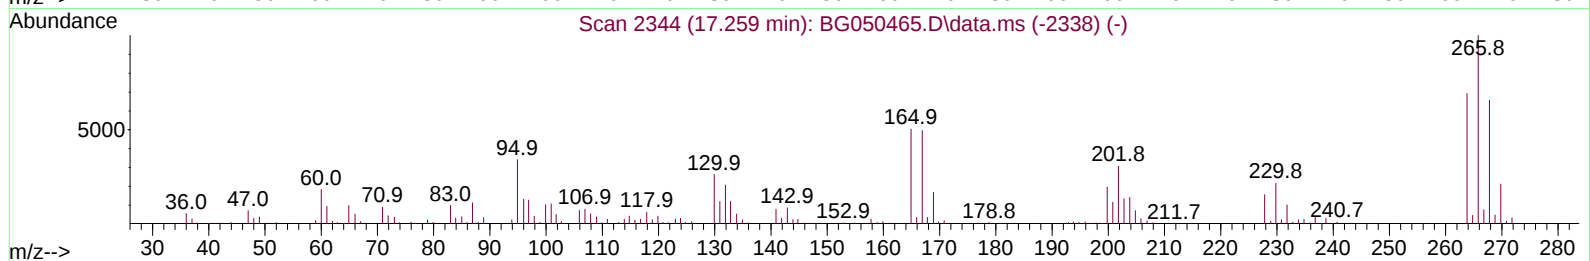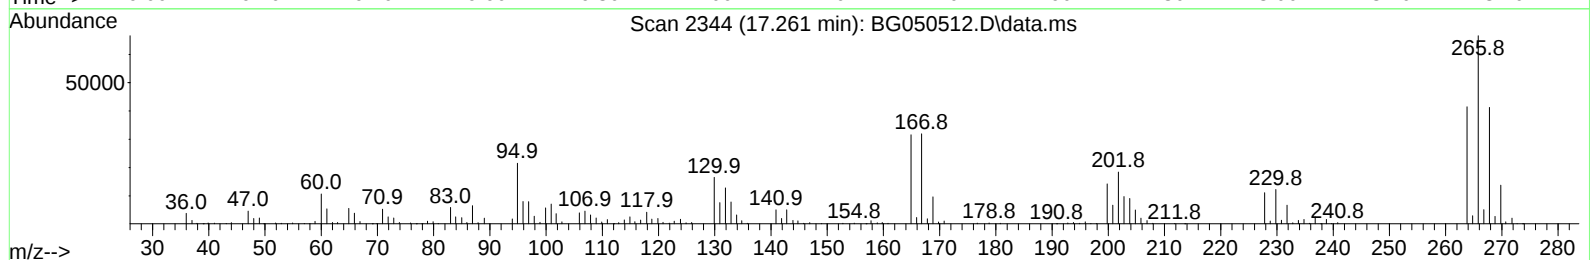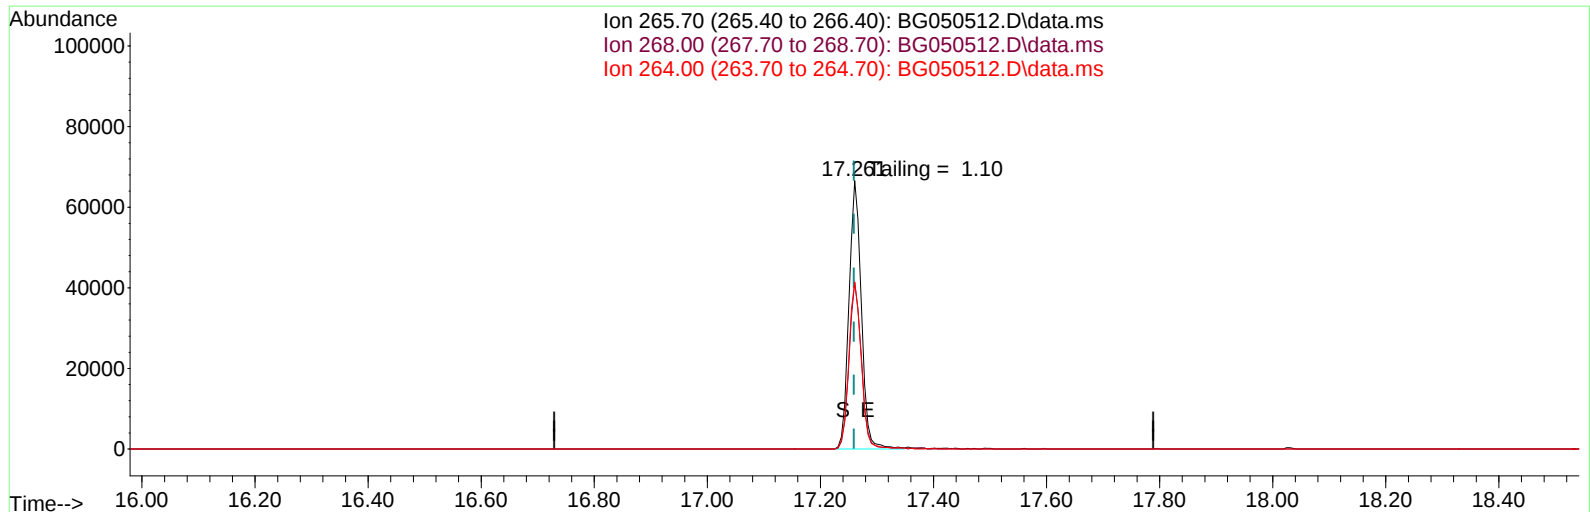

TIC: BG050512.D\data.ms

(70) Pentachlorophenol (C)

17.261min (+ 0.002) 24852.44 ng




response 101325

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.20	61.99
264.00	61.30	62.27
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG100821\
Data File : BG050512.D
Acq On : 8 Oct 2021 16:50
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 09 04:58:18 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100621.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 06 15:51:01 2021
Response via : Initial Calibration

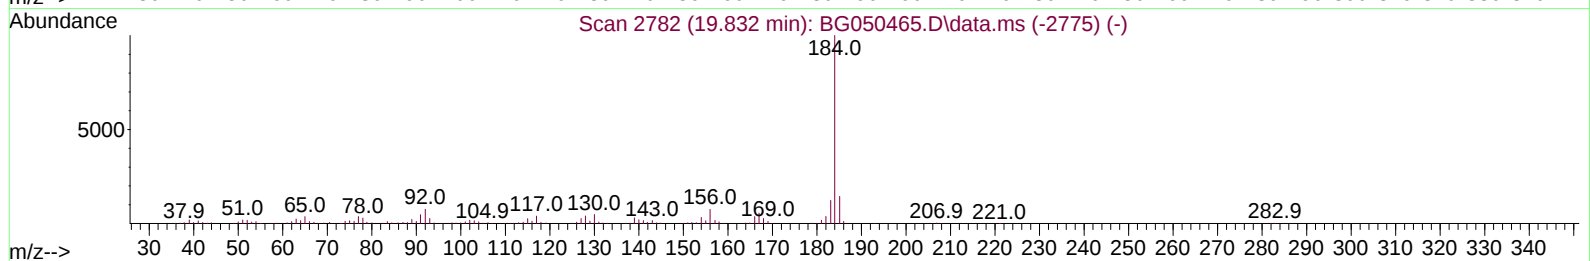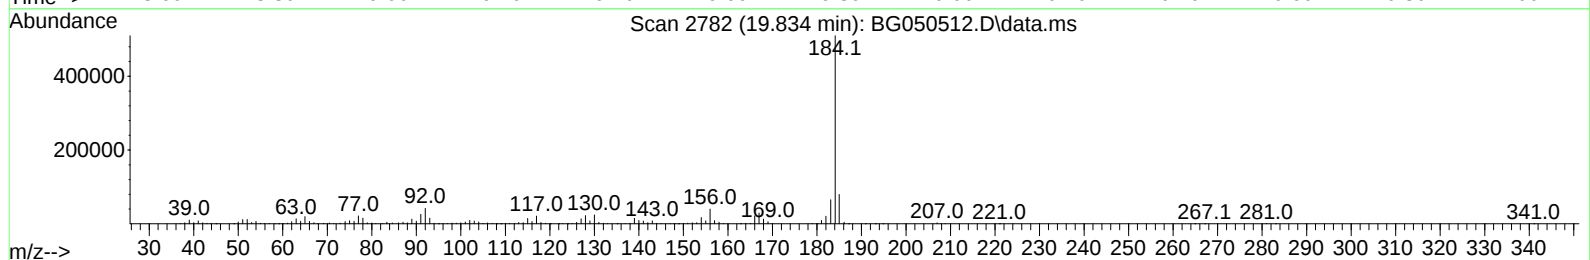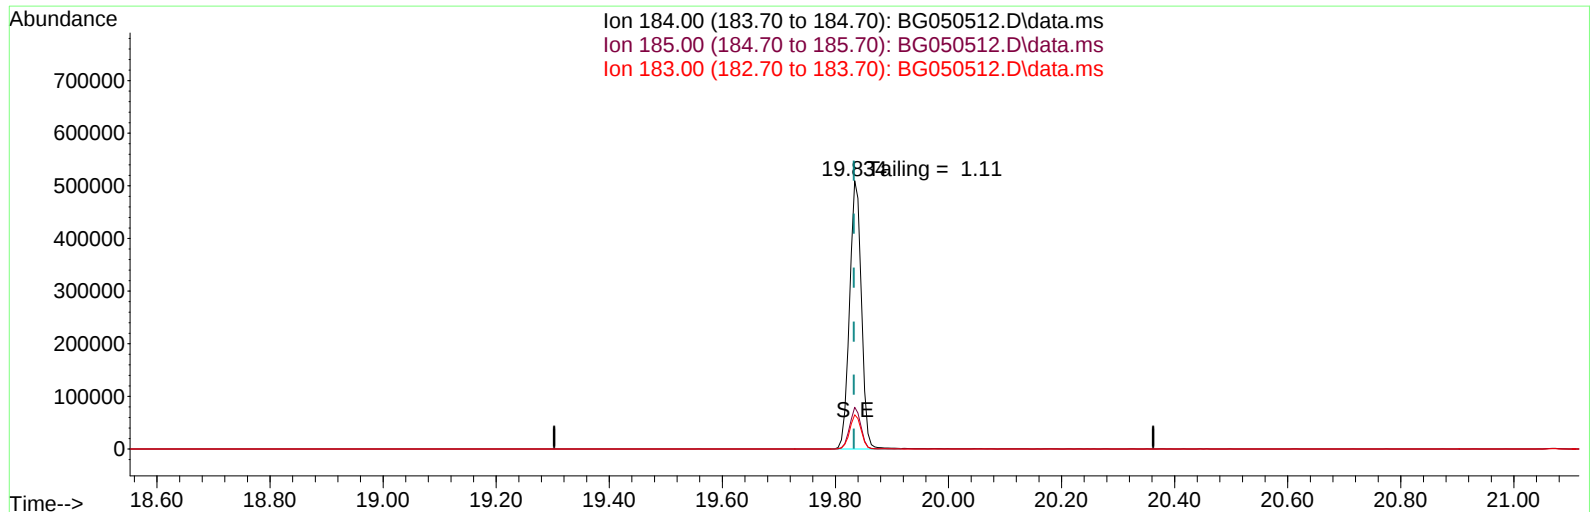

TIC: BG050512.D\data.ms

(77) Benzidine

19.834min (+ 0.002) 425303.09 ng

response 744367

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.40	15.57
183.00	11.70	12.77
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_G
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
10/8/2021	BNA_G	BG050512.D
Compound Name	Response	Retention Time
DDT	319041	21.068
DDD	14310	20.615
DDE	330	20.11
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14640	333681	4.39