

Data Path : Z:\HPCHEM1\BNA_G\Data\BG100915\
 Data File : BG019078.D
 Acq On : 9 Oct 2015 12:42
 Operator : UM/NP
 Sample : PB86031BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Quant Time: Oct 09 18:27:10 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG100415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Oct 09 02:23:12 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.03	152	18720	20.00	ng/ul	0.00
18) Naphthalene-d8	10.84	136	85803	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.67	164	63412	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.41	188	162342	20.00	ng/ul	0.00
78) Chrysene-d12	21.68	240	201204	20.00	ng/ul	0.00
86) Perylene-d12	24.91	264	182320	20.00	ng/ul	-0.01


System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.48	96	2596	6.27	ng/uL	0.00
5) Phenol-d5	7.19	99	55028	34.11	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.36	67	40010	38.33	ng/ul	0.00
9) 2-Chlorophenol-d4	7.57	132	43582	35.99	ng/ul	0.00
13) 4-Methylphenol-d8	8.74	113	48594	38.32	ng/ul	0.00
19) Nitrobenzene-d5	9.20	128	25454	39.24	ng/ul	0.00
22) 2-Nitrophenol-d4	9.92	143	27589	41.34	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.46	165	48522	36.33	ng/ul	0.00
29) 4-Chloroaniline-d4	10.98	131	1014	0.62	ng/ul	0.00
44) Dimethylphthalate-d6	14.07	166	203867	40.78	ng/ul	0.00
47) Acenaphthylene-d8	14.36	160	219708	35.53	ng/ul	0.00
52) 4-Nitrophenol-d4	14.86	143	37874	37.50	ng/ul	0.00
58) Fluorene-d10	15.65	176	168589	37.24	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.77	200	33492	38.03	ng/ul	0.00
71) Anthracene-d10	17.51	188	292082	38.21	ng/ul	0.00
79) Pyrene-d10	19.80	212	370807	39.79	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.70	264	372910	39.98	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
15) N-Nitroso-di-n-propylamine	8.74	70	1160	1.10	ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\Data\BG100915\
Data File : BG019078.D
Acq On : 9 Oct 2015 12:42
Operator : UM/NP
Sample : PB86031BL
Misc :
ALS Vial : 4 Sample Multiplier: 1


Quant Time: Oct 09 18:27:10 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG100415.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Oct 09 02:23:12 2015
Response via : Initial Calibration

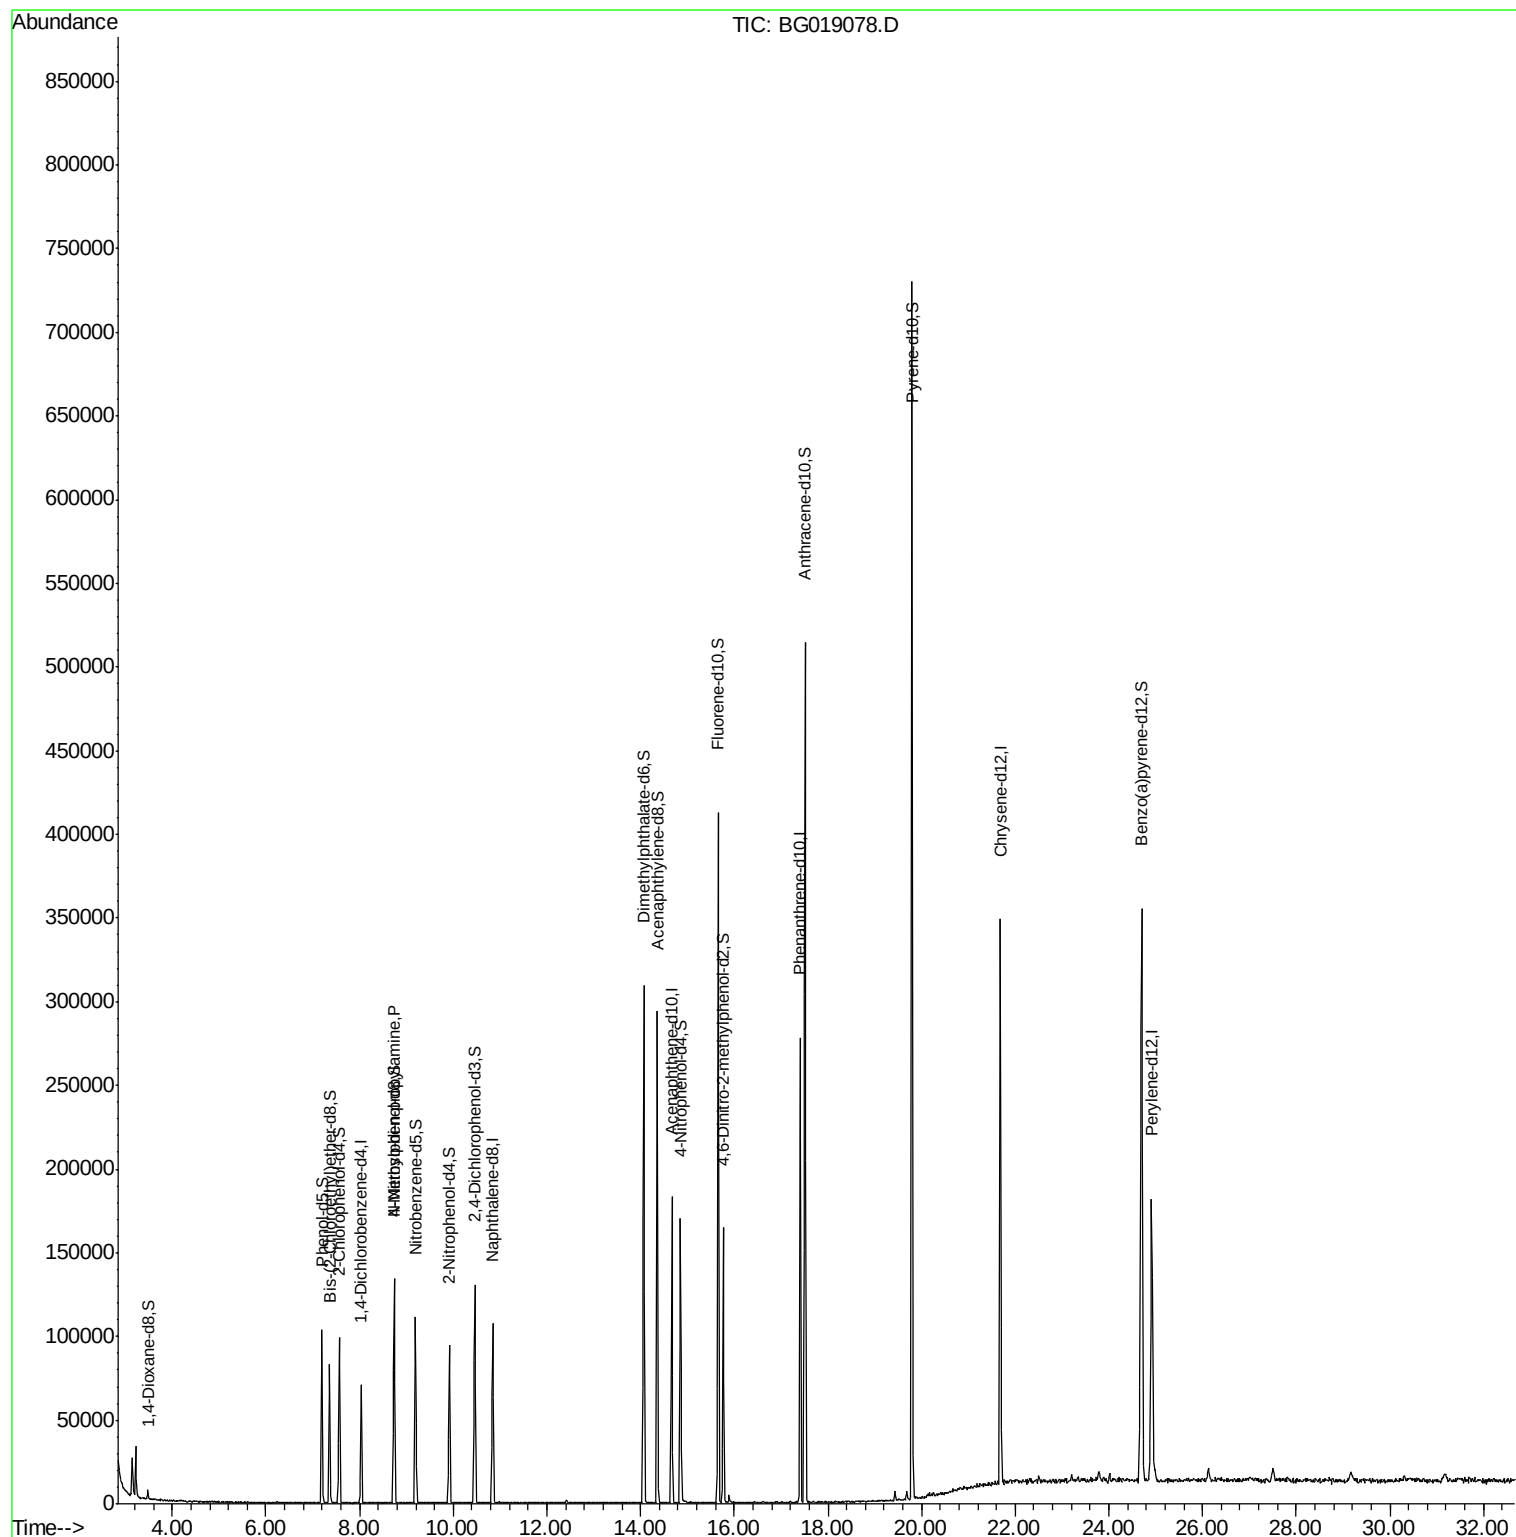

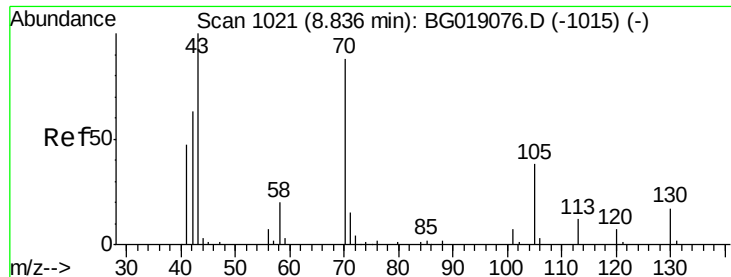

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.10 ng/ul
 RT: 8.74 min Scan# 1004
 Delta R.T. -0.10 min
 Lab File: BG019078.D
 Acq: 9 Oct 2015 12:42

Tgt Ion: 70 Resp: 1160
 Ion Ratio Lower Upper
 70 100
 42 478.4 53.6 80.4#
 101 0.0 7.9 11.9#
 130 0.0 16.5 24.7#

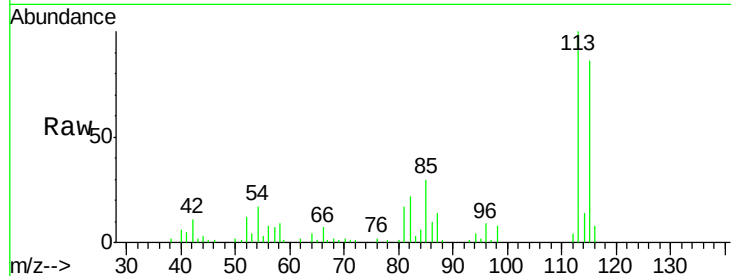

Abundance Ion 70.00 (69.70 to 70.70): BGC
 Ion 42.00 (41.70 to 42.70): BGC
 Ion 101.00 (100.70 to 101.70): BGC
 Ion 130.00 (129.70 to 130.70): BGC

