

Data Path : Z:\HPCHEM1\BNA G\DATA\BG100915\
 Data File : BG019085.D
 Acq On : 9 Oct 2015 18:40
 Operator : UM/NP
 Sample : PB86002BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Quant Time: Oct 10 00:39:19 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG100415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 10 00:37:29 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.04	152	19033	20.00	ng/ul	0.00
18) Naphthalene-d8	10.84	136	88920	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.66	164	59454	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.41	188	152292	20.00	ng/ul	0.00
78) Chrysene-d12	21.68	240	184966	20.00	ng/ul	0.00
86) Perylene-d12	24.91	264	168082	20.00	ng/ul	-0.01


System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.48	96	2206	5.24	ng/uL	0.00
5) Phenol-d5	7.20	99	56319	34.34	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.36	67	39200	36.93	ng/ul	0.00
9) 2-Chlorophenol-d4	7.57	132	45119	36.65	ng/ul	0.00
13) 4-Methylphenol-d8	8.74	113	47987	37.22	ng/ul	0.00
19) Nitrobenzene-d5	9.19	128	23771	35.36	ng/ul	0.00
22) 2-Nitrophenol-d4	9.92	143	27386	39.60	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.46	165	47319	34.19	ng/ul	0.00
29) 4-Chloroaniline-d4	10.98	131	1386	0.82	ng/ul	0.00
44) Dimethylphthalate-d6	14.07	166	191805	40.92	ng/ul	0.00
47) Acenaphthylene-d8	14.35	160	210480	36.30	ng/ul	0.00
52) 4-Nitrophenol-d4	14.85	143	34609	36.55	ng/ul	0.00
58) Fluorene-d10	15.65	176	159980	37.69	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.76	200	29430	35.62	ng/ul	0.00
71) Anthracene-d10	17.51	188	265428	37.01	ng/ul	0.00
79) Pyrene-d10	19.80	212	327494	38.23	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.70	264	327474	38.08	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
15) N-Nitroso-di-n-propylamine	8.74	70	1318	1.23	ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG100915\
Data File : BG019085.D
Acq On : 9 Oct 2015 18:40
Operator : UM/NP
Sample : PB86002BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Quant Time: Oct 10 00:39:19 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG100415.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 10 00:37:29 2015
Response via : Initial Calibration

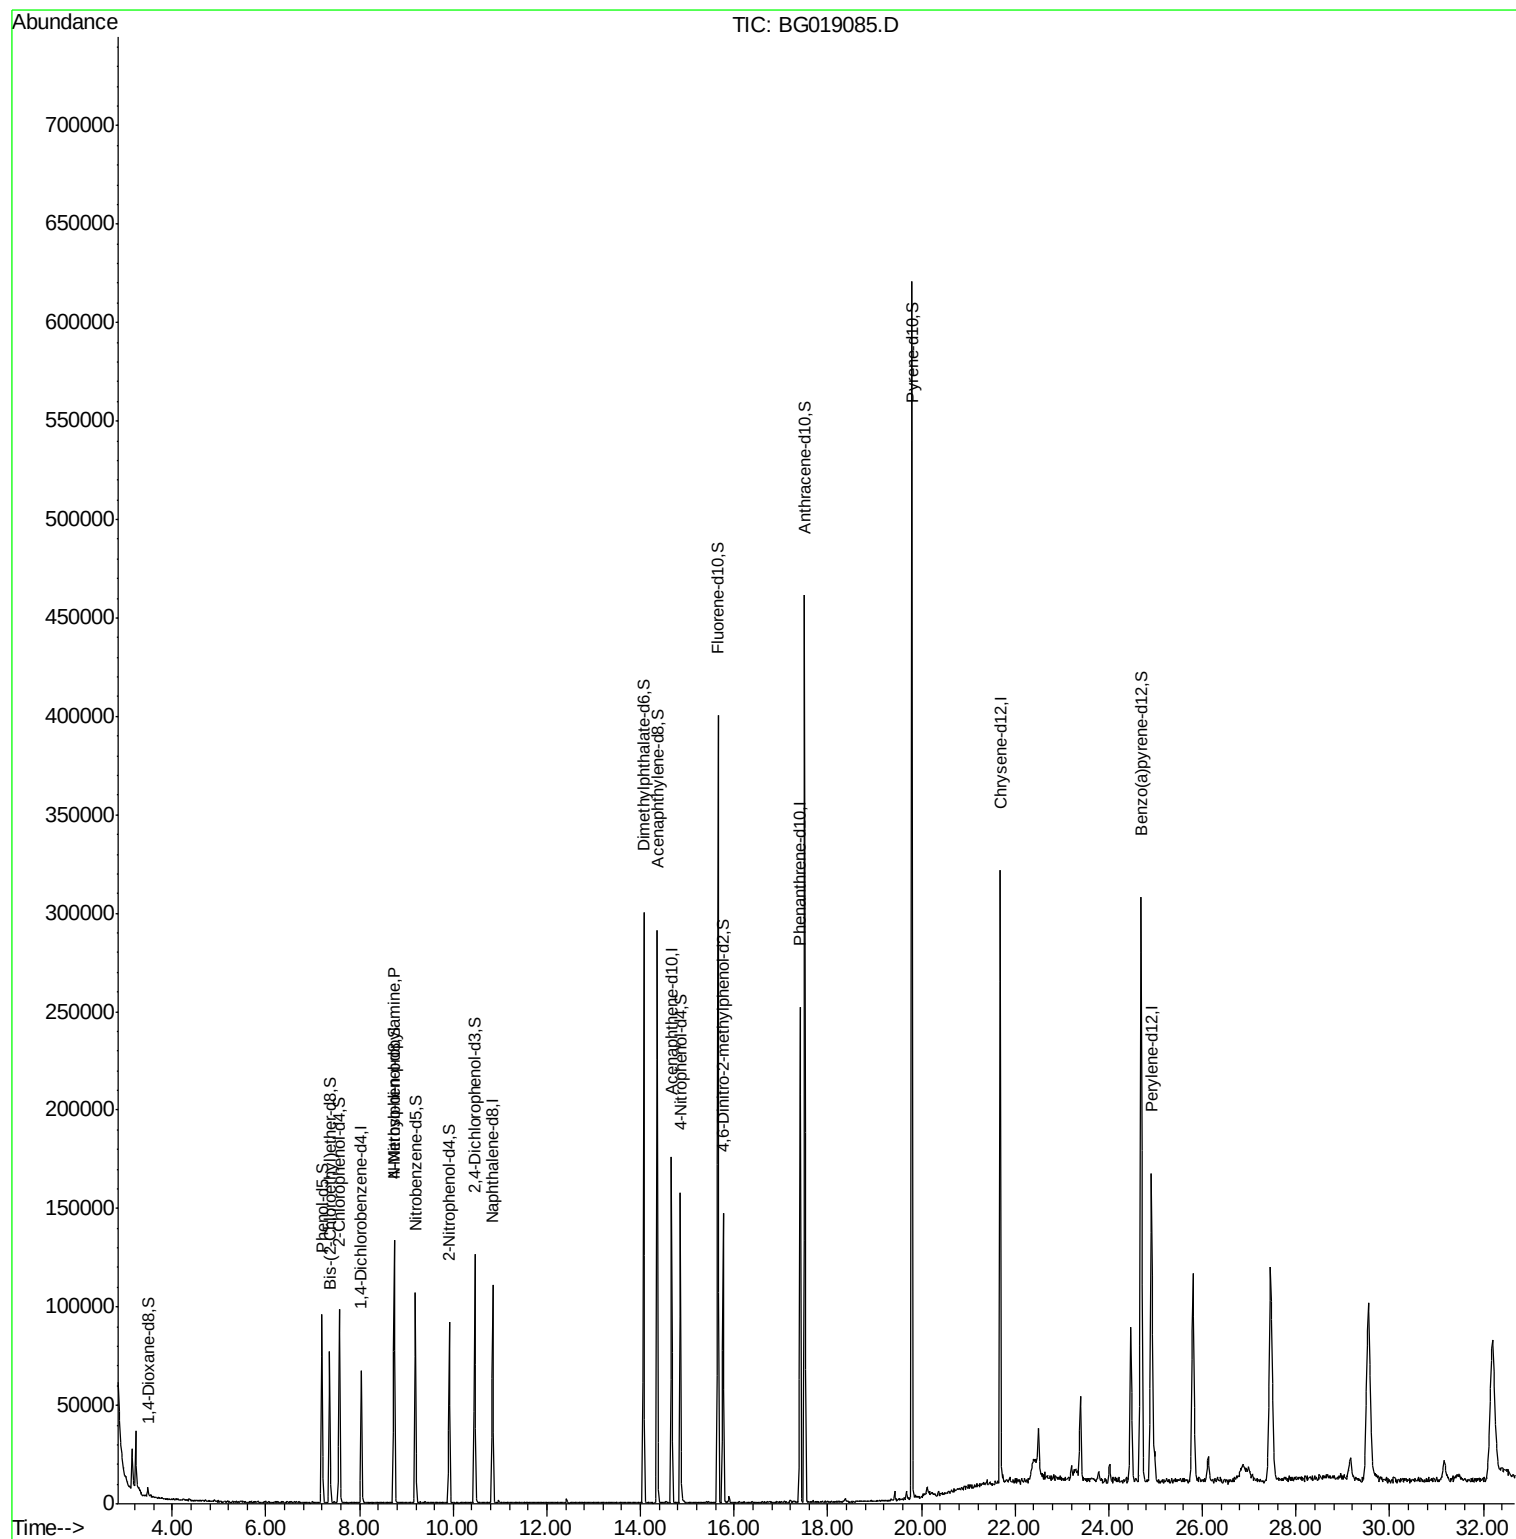

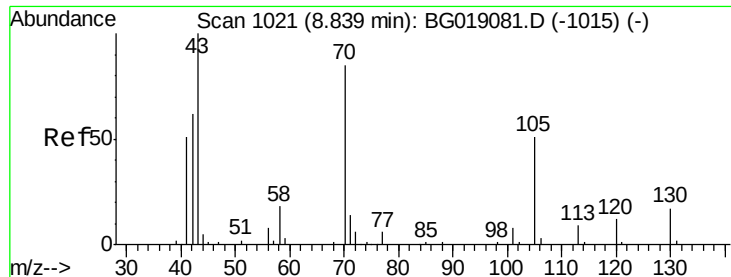

#15
 N-Nitroso-di-n-propylamine
 Concen: 1.23 ng/ul
 RT: 8.74 min Scan# 1005
 Delta R.T. -0.10 min
 Lab File: BG019085.D
 Acq: 9 Oct 2015 18:40

Tot Ion:	70	Resp:	1318
Ion	Ratio	Lower	Upper
70	100		
42	386.3	53.6	80.4#
101	0.0	7.9	11.9#
130	0.0	16.5	24.7#

