

Data Path : Z:\HPCHEM1\BNA G\DATA\BG100915\
 Data File : BG019092.D
 Acq On : 9 Oct 2015 23:07
 Operator : UM/NP
 Sample : G3966-12
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Quant Time: Oct 10 00:40:21 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG100415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 10 00:37:29 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.04	152	18204	20.00	ng/ul	0.00
18) Naphthalene-d8	10.84	136	83853	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.66	164	58880	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.41	188	149479	20.00	ng/ul	0.00
78) Chrysene-d12	21.68	240	187226	20.00	ng/ul	0.00
86) Perylene-d12	24.91	264	177915	20.00	ng/ul	-0.02


System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.48	96	339	0.84	ng/uL	0.00
5) Phenol-d5	7.20	99	11919	7.60	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.36	67	33668	33.17	ng/ul	0.00
9) 2-Chlorophenol-d4	7.57	132	32282	27.42	ng/ul	0.00
13) 4-Methylphenol-d8	8.74	113	24023	19.48	ng/ul	0.00
19) Nitrobenzene-d5	9.19	128	21751	34.31	ng/ul	0.00
22) 2-Nitrophenol-d4	9.92	143	24803	38.03	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.46	165	44979	34.46	ng/ul	0.00
29) 4-Chloroaniline-d4	11.00	131	1089	0.68	ng/ul	0.02
44) Dimethylphthalate-d6	14.07	166	170912	36.81	ng/ul	0.00
47) Acenaphthylene-d8	14.36	160	193125	33.63	ng/ul	0.00
52) 4-Nitrophenol-d4	14.85	143	6901	7.36	ng/ul	0.00
58) Fluorene-d10	15.65	176	152307	36.24	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.76	200	29838	36.80	ng/ul	0.00
71) Anthracene-d10	17.51	188	247613	35.18	ng/ul	0.00
79) Pyrene-d10	19.79	212	307473	35.46	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.69	264	327899	36.02	ng/ul	-0.01


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
17) Hexachloroethane	9.22	117	1341	2.76	ng/ul#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG100915\
Data File : BG019092.D
Acq On : 9 Oct 2015 23:07
Operator : UM/NP
Sample : G3966-12
Misc :
ALS Vial : 18 Sample Multiplier: 1

Quant Time: Oct 10 00:40:21 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG100415.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 10 00:37:29 2015
Response via : Initial Calibration

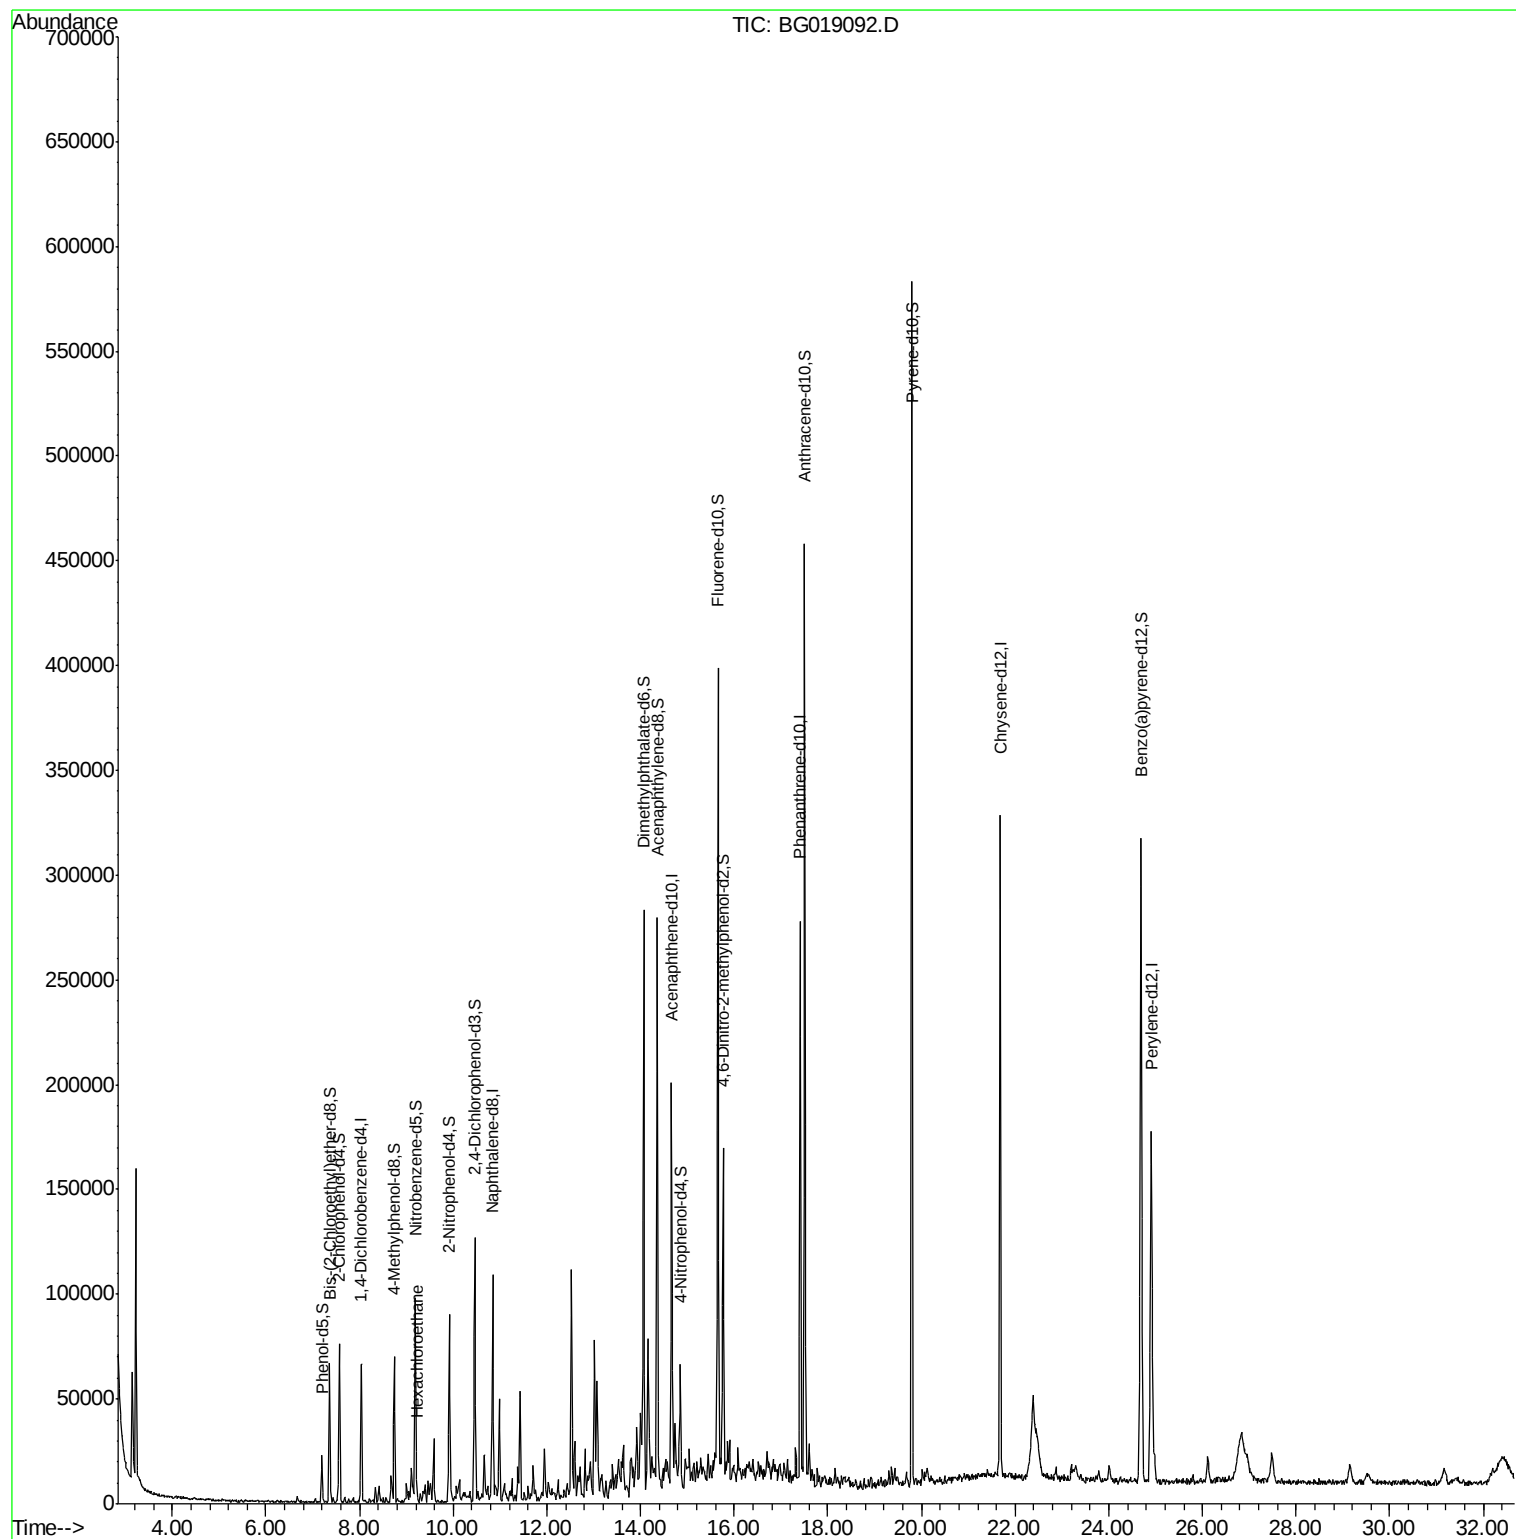

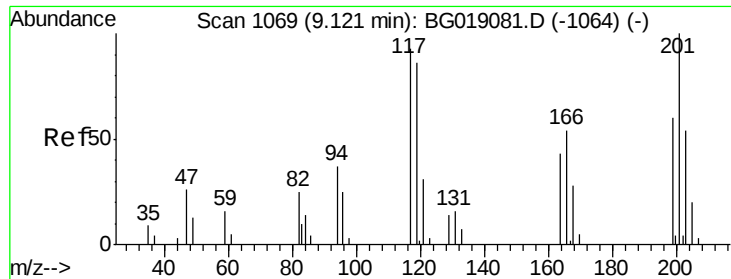

#17

Hexachloroethane

Concen: 2.76 ng/ul

RT: 9.22 min Scan# 1087

Delta R.T. 0.10 min

Lab File: BG019092.D

Acq: 9 Oct 2015 23:07


Tot Ion:117 Resp: 1341

Ion Ratio Lower Upper

117 100

201 0.0 91.4 137.0#

199 0.0 58.7 88.1#

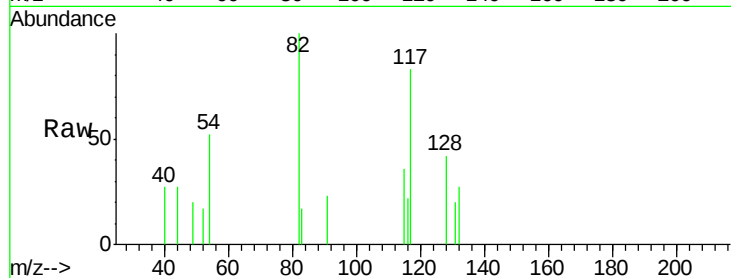

Abundance Ion 117.00 (116.70 to 117.70): E

Ion 201.00 (200.70 to 201.70): E

Ion 199.00 (198.70 to 199.70): E

