

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG100915\
 Data File : BG019084.D
 Acq On : 9 Oct 2015 18:02
 Operator : UM/NP
 Sample : G3966-02
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E5LE5

Quant Time: Oct 10 00:39:10 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG100415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 10 00:37:29 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.04	152	18884	20.00	ng/ul	0.00
18) Naphthalene-d8	10.84	136	88638	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.66	164	63792	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.41	188	167687	20.00	ng/ul	0.00
78) Chrysene-d12	21.68	240	214501	20.00	ng/ul	0.00
86) Perylene-d12	24.92	264	201593	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.48	96	500	1.20	ng/uL	0.00
5) Phenol-d5	7.20	99	12015	7.38	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.36	67	29951	28.44	ng/ul	0.00
9) 2-Chlorophenol-d4	7.57	132	29469	24.13	ng/ul	0.00
13) 4-Methylphenol-d8	8.73	113	22559	17.63	ng/ul	-0.01
19) Nitrobenzene-d5	9.19	128	19397	28.94	ng/ul	0.00
22) 2-Nitrophenol-d4	9.92	143	21913	31.79	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.46	165	39654	28.74	ng/ul	0.00
29) 4-Chloroaniline-d4	10.98	131	1939	1.15	ng/ul	0.00
44) Dimethylphthalate-d6	14.07	166	159272	31.67	ng/ul	0.00
47) Acenaphthylene-d8	14.36	160	174426	28.04	ng/ul	0.00
52) 4-Nitrophenol-d4	14.86	143	8031	7.90	ng/ul	0.00
58) Fluorene-d10	15.66	176	137175	30.12	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.77	200	28614	31.46	ng/ul	0.00
71) Anthracene-d10	17.51	188	241831	30.63	ng/ul	0.00
79) Pyrene-d10	19.79	212	306068	30.81	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.70	264	319327	30.96	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.11	163	16926	3.30	ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG100915\
Data File : BG019084.D
Acq On : 9 Oct 2015 18:02
Operator : UM/NP
Sample : G3966-02
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E5LE5

Quant Time: Oct 10 00:39:10 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG100415.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 10 00:37:29 2015
Response via : Initial Calibration

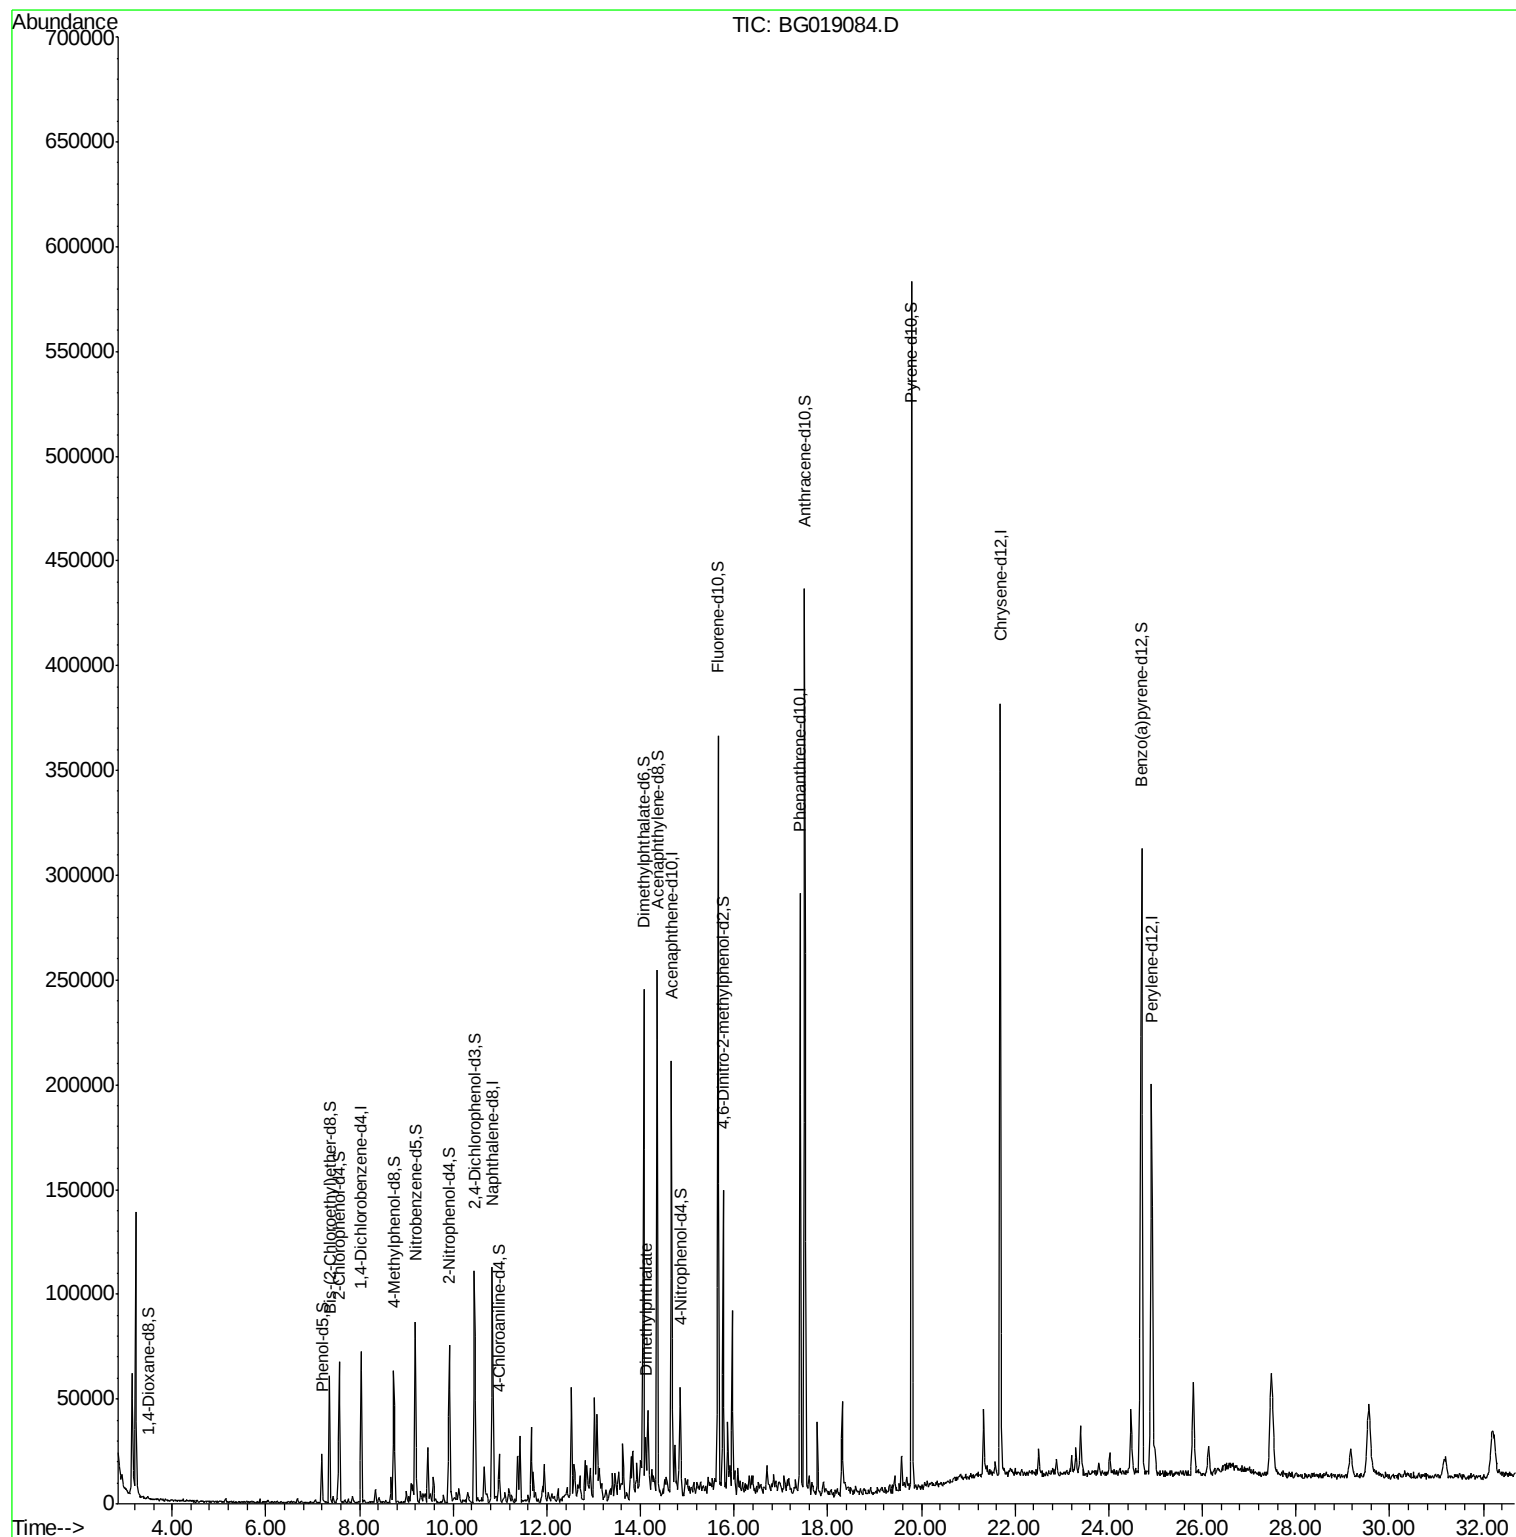

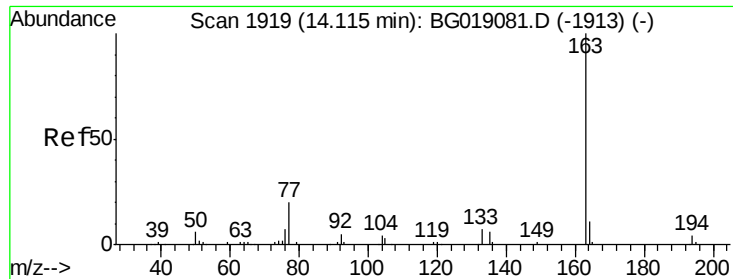

#45

Dimethylphthalate

Concen: 3.30 ng/ul

RT: 14.11 min Scan# 1918

Delta R.T. -0.00 min

Lab File: BG019084.D


Acq: 9 Oct 2015 18:02

Instrument :

BNA_G

ClientSampleId :

E5LE5

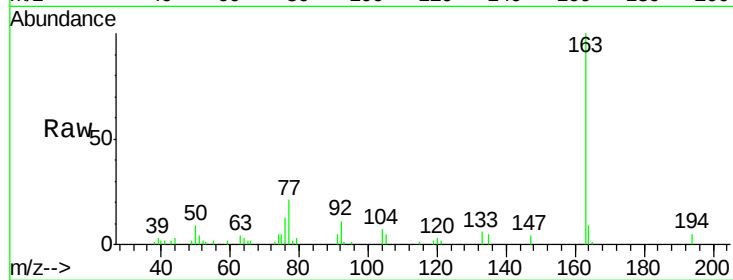

Tgt Ion:	163	Resp:	16926
Ion	Ratio	Lower	Upper
163	100		
194	4.6	3.3	4.9
164	8.8	8.1	12.1

