

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG100915\
 Data File : BG019093.D
 Acq On : 9 Oct 2015 23:45
 Operator : UM/NP
 Sample : G3966-10
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 E5LF7

Quant Time: Oct 10 00:40:29 2015
 Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG100415.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Oct 10 00:37:29 2015
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.03	152	17277	20.00	ng/ul	0.00
18) Naphthalene-d8	10.84	136	77258	20.00	ng/ul	0.00
36) Acenaphthene-d10	14.66	164	56073	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.41	188	146597	20.00	ng/ul	0.00
78) Chrysene-d12	21.68	240	177745	20.00	ng/ul	-0.01
86) Perylene-d12	24.91	264	170351	20.00	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.48	96	180	0.47	ng/uL	0.00
5) Phenol-d5	7.19	99	5546	3.72	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.36	67	18179	18.87	ng/ul	0.00
9) 2-Chlorophenol-d4	7.56	132	17070	15.27	ng/ul	0.00
13) 4-Methylphenol-d8	8.73	113	11634	9.94	ng/ul	-0.01
19) Nitrobenzene-d5	9.19	128	11618	19.89	ng/ul	0.00
22) 2-Nitrophenol-d4	9.91	143	13421	22.34	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.46	165	22718	18.89	ng/ul	0.00
29) 4-Chloroaniline-d4	10.97	131	468	0.32	ng/ul	0.00
44) Dimethylphthalate-d6	14.06	166	99358	22.47	ng/ul	0.00
47) Acenaphthylene-d8	14.36	160	109354	20.00	ng/ul	0.00
52) 4-Nitrophenol-d4	14.85	143	2600	2.91	ng/ul	0.00
58) Fluorene-d10	15.65	176	84045	21.00	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.76	200	14907	18.75	ng/ul	-0.01
71) Anthracene-d10	17.51	188	144425	20.92	ng/ul	0.00
79) Pyrene-d10	19.79	212	178727	21.71	ng/ul	0.00
90) Benzo(a)pyrene-d12	24.69	264	183072	21.00	ng/ul	-0.02


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
45) Dimethylphthalate	14.11	163	27394	6.07	ng/ul#	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_G\DATA\BG100915\
Data File : BG019093.D
Acq On : 9 Oct 2015 23:45
Operator : UM/NP
Sample : G3966-10
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
E5LF7

Quant Time: Oct 10 00:40:29 2015
Quant Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG100415.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Oct 10 00:37:29 2015
Response via : Initial Calibration

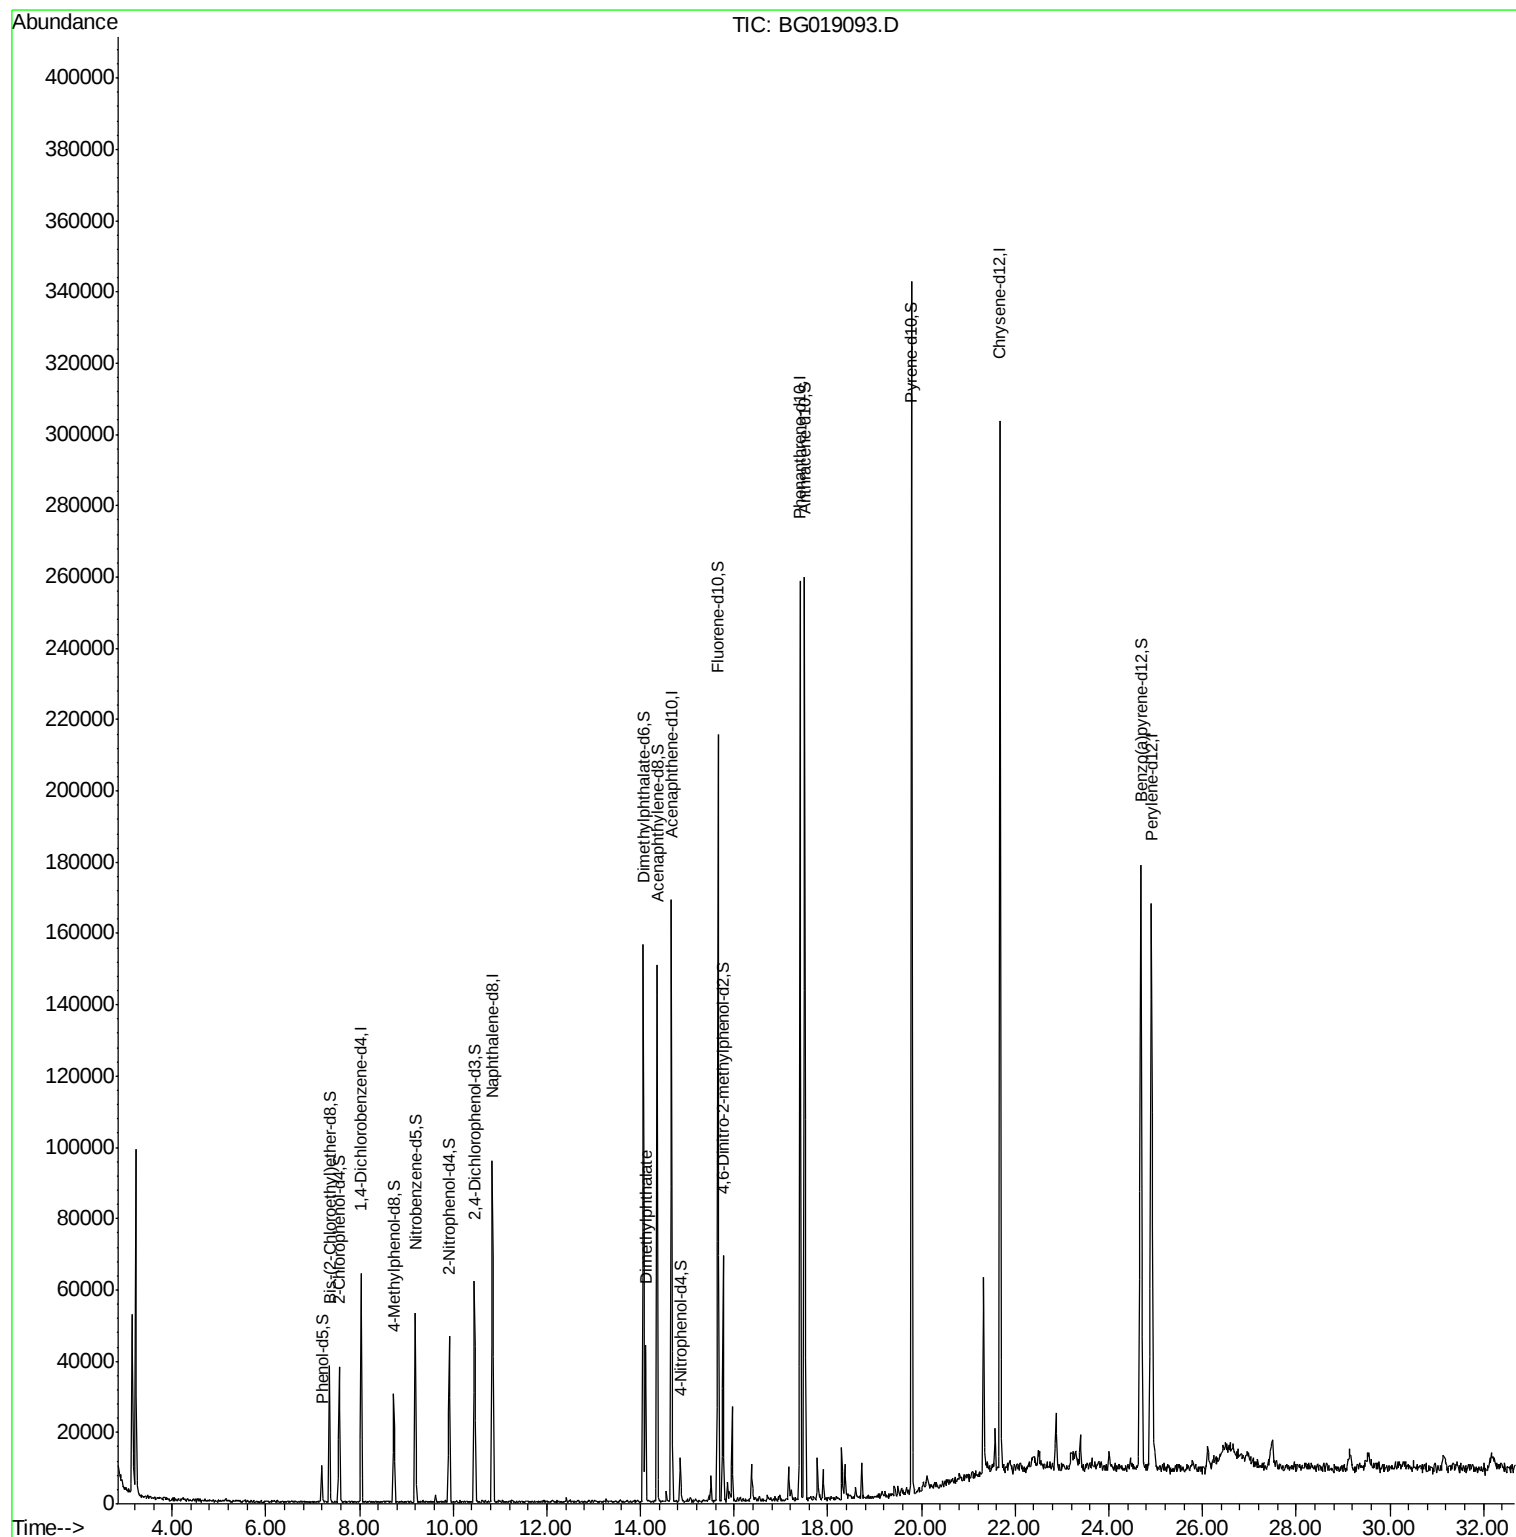

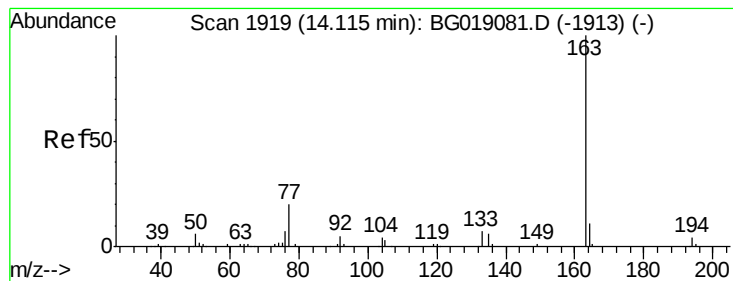

#45

Dimethylphthalate

Concen: 6.07 ng/ul

RT: 14.11 min Scan# 1918

Delta R.T. -0.01 min

Lab File: BG019093.D


Acq: 9 Oct 2015 23:45

Instrument :

BNA_G

ClientSampleId :

E5LF7

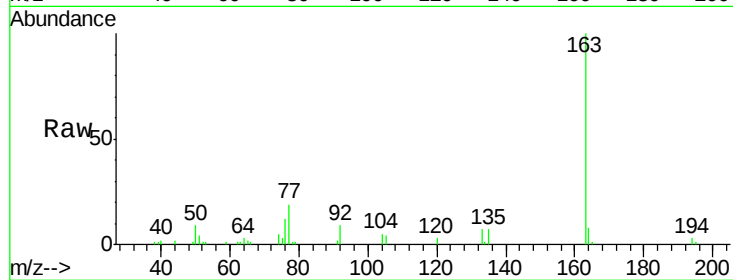

Tgt Ion:	163	Resp:	27394
Ion	Ratio	Lower	Upper
163	100		
194	2.8	3.3	4.9#
164	8.4	8.1	12.1

