


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG100915\
Data File : BG019075.D
Acq On : 9 Oct 2015 8:40
Operator : UM/NP
Sample : DFTPP64
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP64

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_G\METHODS\SOM02.2-EPA-BG100415.M
Title : SVOA CALIBRATION
Last Update : Mon Oct 12 15:15:32 2015

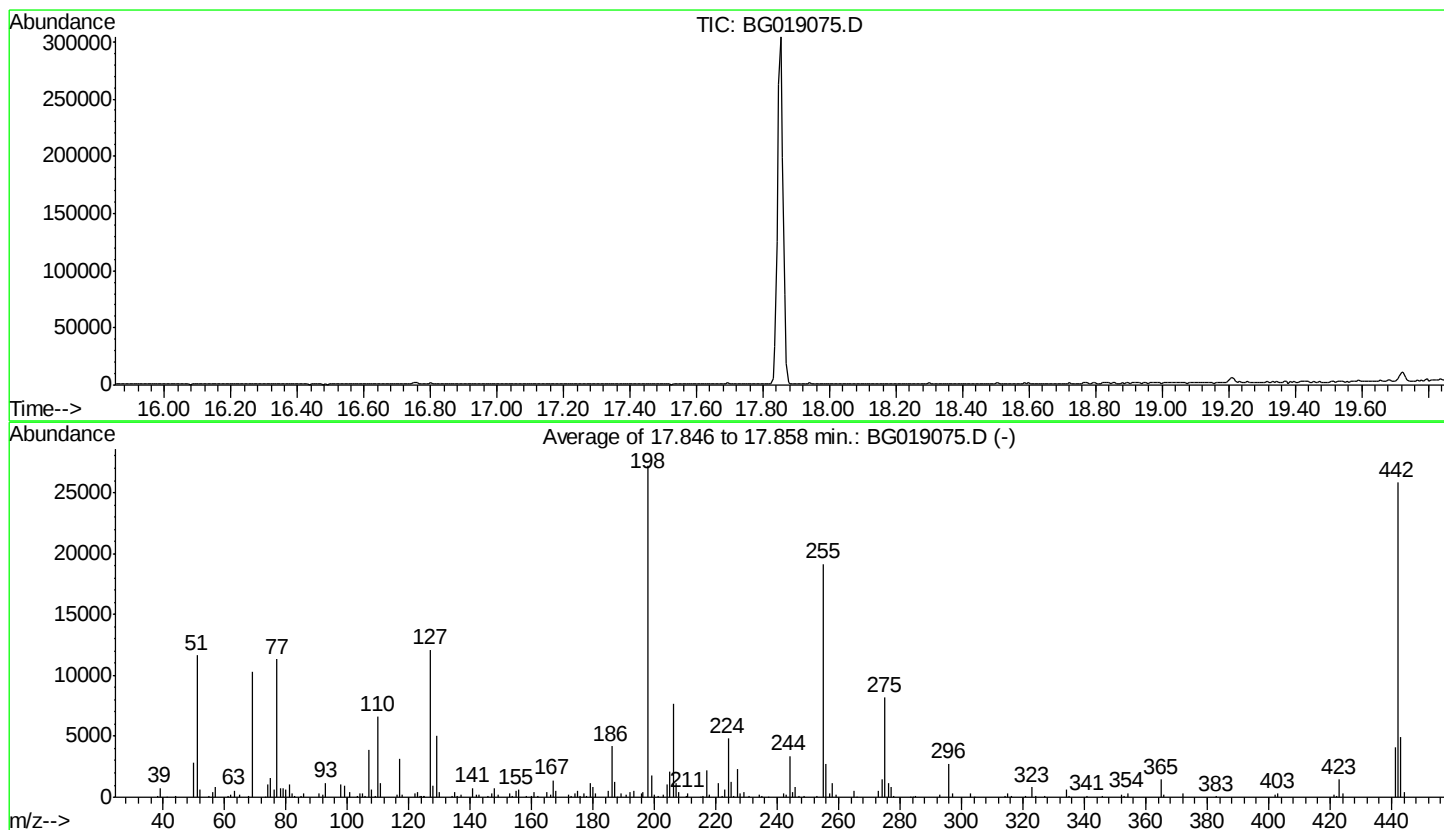

AutoFind: Scans 2554, 2555, 2556; Background Corrected with Scan 2549

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.7	11631	PASS
68	69	0.00	2	1.3	132	PASS
69	198	0.00	100	38.0	10345	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.5	12112	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	27210	PASS
199	198	5	9	6.7	1815	PASS
275	198	10	60	30.0	8164	PASS
365	198	1	100	5.3	1438	PASS
441	442	0.01	24	15.8	4074	PASS
442	198	50	100	94.9	25826	PASS
443	442	15	24	19.2	4948	PASS

m/z	Abundance
38.10	214.0
39.10	1071.0
40.00	379.0
41.00	161.0
44.00	493.0
50.10	3211.0
51.10	14259.0
52.10	721.0
56.00	432.0
57.00	901.0
61.10	184.0
62.10	236.0
63.10	675.0
65.00	376.0
69.00	12315.0
73.10	151.0
74.10	1286.0
75.00	1831.0
76.10	858.0
77.10	13418.0
78.10	1008.0
79.10	698.0
80.10	784.0
81.00	1078.0
82.00	379.0
83.00	162.0
86.00	427.0
90.90	256.0
92.00	252.0
93.00	1289.0
98.00	1270.0
99.00	913.0
101.00	486.0
104.00	398.0
105.00	274.0
106.00	173.0
107.00	4280.0
108.00	735.0
109.00	208.0
110.00	7718.0
111.00	1194.0
116.00	265.0
117.00	3530.0
118.10	202.0
122.10	348.0
123.00	611.0
123.90	195.0
124.90	272.0
127.10	12932.0
128.10	1157.0
129.00	5808.0
130.00	412.0
133.90	243.0
135.10	532.0
137.00	361.0
141.00	753.0
142.00	267.0
143.00	197.0
146.00	196.0
147.00	235.0
148.00	685.0
149.00	281.0
153.10	445.0
155.00	547.0
156.00	846.0
158.20	249.0
161.00	568.0
161.90	216.0
165.00	432.0
166.10	262.0
167.00	1386.0
168.00	651.0
172.00	193.0
173.00	185.0
174.00	339.0
175.10	431.0
177.00	231.0
179.00	1279.0
180.00	805.0
181.00	405.0
185.10	703.0
186.00	4336.0
187.00	1200.0
188.00	159.0
189.00	392.0
190.90	270.0
192.00	407.0
193.10	531.0
195.90	888.0
198.00	28128.0
198.90	1733.0

Instrument :
BNA_G
ClientSampleId :
DFTPP64

200.00	277.0
201.40	203.0
202.90	282.0
204.00	1123.0
205.10	2395.0
206.10	8006.0
207.00	1327.0
208.00	285.0
211.00	306.0
216.00	220.0
217.00	2269.0
217.90	312.0
221.00	1040.0
223.00	716.0
224.00	5151.0
225.00	1236.0
225.90	167.0
227.00	2458.0
228.00	400.0
229.00	392.0
234.00	219.0
242.00	366.0
243.10	306.0
244.10	3380.0
245.10	458.0
246.00	950.0
247.00	243.0
253.10	182.0
255.00	18208.0
256.00	2591.0
257.00	234.0
258.00	1184.0
258.90	232.0
265.00	389.0
273.00	546.0
274.00	1473.0
275.00	7520.0
276.00	999.0
277.00	886.0
278.00	208.0
293.00	162.0
296.00	2467.0
297.00	469.0
303.00	401.0
304.10	162.0
315.00	320.0
323.00	628.0
326.90	171.0
334.10	565.0
335.00	164.0
341.00	230.0
345.90	151.0
352.10	288.0
354.00	282.0
365.00	1189.0
365.90	227.0
372.00	373.0
403.00	211.0
421.10	182.0
423.00	1118.0
423.90	171.0
441.10	3200.0
442.00	20672.0
443.10	4259.0
444.00	444.0

Instrument :
BNA_G
ClientSampleId :
DFTPP64

m/z	Abundance
39.10	728.0
40.00	313.0
44.00	553.0
50.10	3193.0
51.10	12926.0
52.10	692.0
55.10	221.0
56.10	423.0
57.10	1081.0
61.10	219.0
62.00	192.0
63.10	597.0
65.10	225.0
68.00	244.0
69.00	11543.0
74.00	1016.0
75.00	1821.0
76.10	753.0
77.10	12489.0
78.10	903.0
79.00	856.0
80.00	763.0
81.00	1379.0
82.10	297.0
83.00	287.0
85.10	272.0
86.00	335.0
91.00	429.0
92.00	258.0
93.00	1447.0
98.10	1156.0
99.00	1122.0
101.00	587.0
103.10	276.0
104.00	366.0
105.00	336.0
107.10	4512.0
108.00	633.0
110.00	7401.0
111.00	1461.0
116.00	282.0
117.00	3675.0
118.00	266.0
122.00	318.0
123.00	461.0
124.10	245.0
125.10	211.0
127.10	14498.0
128.00	1112.0
129.00	6017.0
130.00	510.0
134.00	182.0
135.10	558.0
136.00	190.0
137.10	261.0
141.00	1140.0
142.10	330.0
143.00	182.0
147.10	502.0
148.00	1026.0
149.00	255.0
152.90	200.0
153.90	223.0
155.00	748.0
156.00	758.0
158.00	166.0
160.10	277.0
161.00	465.0
165.00	462.0
166.00	353.0
167.00	1811.0
168.00	633.0
172.00	191.0
173.00	282.0
174.00	432.0
175.00	804.0
175.80	240.0
177.00	399.0
177.80	220.0
179.00	1217.0
180.00	1018.0
180.90	312.0
184.90	482.0
186.00	4810.0
187.00	1576.0
189.00	395.0
191.00	245.0
192.10	577.0
193.10	570.0
196.10	958.0
198.00	32872.0

Instrument :
BNA_G
ClientSampleId :
DFTPP64

199.00	2316.0
203.00	473.0
204.00	1241.0
205.10	2084.0
206.10	9080.0
207.00	1471.0
208.10	501.0
210.20	217.0
211.00	356.0
215.90	213.0
217.00	2663.0
218.10	365.0
221.00	1271.0
221.90	270.0
223.00	675.0
224.00	5774.0
225.00	1680.0
226.00	176.0
227.00	2531.0
228.00	337.0
229.00	400.0
231.00	273.0
234.00	270.0
235.00	196.0
237.00	152.0
242.00	306.0
244.10	3710.0
245.10	533.0
246.00	740.0
248.90	185.0
253.00	175.0
255.00	22864.0
256.00	3348.0
257.10	371.0
258.10	1435.0
259.00	283.0
265.00	708.0
266.00	164.0
273.00	586.0
274.00	1640.0
275.00	10367.0
276.00	1621.0
277.00	928.0
278.00	198.0
283.10	157.0
284.00	161.0
285.10	221.0
293.00	342.0
296.00	3665.0
296.90	396.0
303.00	373.0
314.00	231.0
315.00	432.0
316.10	208.0
321.00	296.0
323.10	1059.0
324.00	232.0
327.00	164.0
334.00	832.0
334.90	192.0
340.90	153.0
346.00	220.0
352.00	291.0
353.00	323.0
354.00	436.0
365.00	1854.0
366.00	154.0
372.00	380.0
383.00	153.0
402.00	267.0
403.00	295.0
421.10	326.0
422.00	228.0
423.00	1701.0
424.00	281.0
441.00	5034.0
442.00	31416.0
443.00	5880.0
444.00	551.0

Instrument :
BNA_G
ClientSampleId :
DFTPP64

m/z	Abundance
39.10	550.0
40.00	311.0
44.00	385.0
50.10	2075.0
51.10	7709.0
52.10	439.0
56.00	321.0
57.00	544.0
62.10	203.0
63.10	364.0
68.10	152.0
69.00	7178.0
74.00	804.0
75.10	1142.0
76.10	408.0
77.10	8026.0
78.10	442.0
79.00	548.0
80.00	455.0
81.10	555.0
82.00	163.0
85.90	155.0
91.00	206.0
93.00	891.0
98.00	735.0
99.00	823.0
101.00	279.0
104.10	207.0
105.00	293.0
107.00	2981.0
108.10	390.0
110.00	4651.0
111.00	753.0
116.10	208.0
117.00	2206.0
118.00	186.0
121.90	274.0
123.00	209.0
124.00	226.0
127.00	8906.0
128.00	663.0
129.00	3202.0
130.00	242.0
135.10	334.0
141.00	385.0
143.00	156.0
147.10	339.0
148.00	494.0
153.10	178.0
155.00	333.0
156.00	418.0
160.00	155.0
161.00	254.0
165.00	342.0
166.10	164.0
167.00	908.0
168.00	315.0
172.00	190.0
174.00	336.0
175.00	495.0
177.10	258.0
179.00	878.0
180.10	619.0
181.10	226.0
185.00	362.0
186.10	3406.0
187.00	897.0
189.00	166.0
191.00	227.0
192.10	313.0
193.10	528.0
196.00	434.0
198.00	20632.0
199.00	1397.0
200.00	215.0
204.10	904.0
205.10	1721.0
206.00	5945.0
207.10	1108.0
208.00	418.0
211.00	330.0
215.10	155.0
217.00	1822.0
218.00	183.0
221.00	1027.0
221.90	165.0
223.00	550.0
224.00	3564.0
225.10	1025.0
227.00	1956.0
228.10	235.0

Instrument :
BNA_G
ClientSampleId :
DFTPP64

228.90	333.0
242.10	227.0
243.00	221.0
244.10	2999.0
245.10	416.0
245.90	749.0
248.90	201.0
255.00	16333.0
256.00	2295.0
256.90	198.0
258.00	786.0
259.00	162.0
265.00	382.0
272.90	560.0
274.10	1449.0
275.00	6607.0
276.10	971.0
277.00	739.0
285.00	154.0
293.00	179.0
296.00	2081.0
297.10	194.0
303.00	319.0
315.10	256.0
323.00	724.0
334.00	548.0
352.00	156.0
353.00	156.0
354.00	381.0
365.00	1273.0
366.00	390.0
372.00	321.0
383.00	161.0
401.90	274.0
403.10	362.0
421.10	272.0
422.10	225.0
423.00	1457.0
424.00	347.0
441.10	3989.0
442.00	25392.0
443.00	4705.0
444.00	413.0

Instrument :
BNA_G
ClientSampleId :
DFTPP64

Scan 2549 (17.817 min): BG019075.D
DFTPP64

m/z	Abundance
40.00	366.0
44.00	364.0
207.00	177.0

Instrument :
BNA_G
ClientSampleId :
DFTPP64