
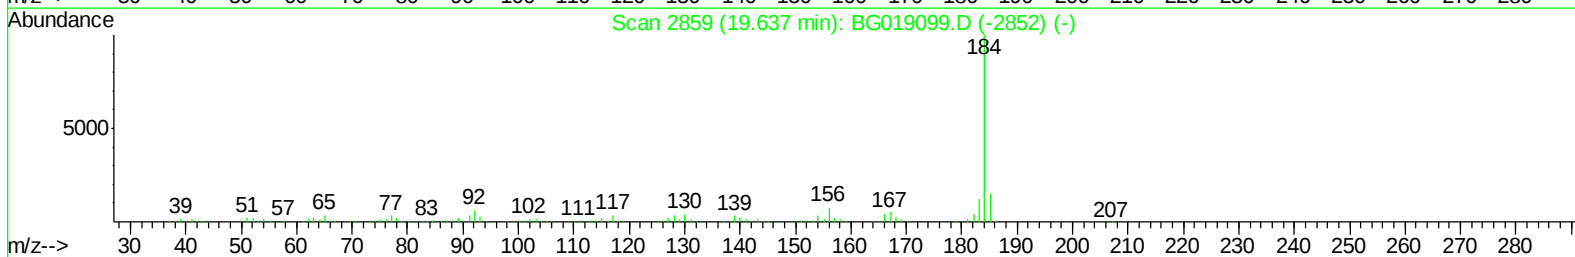
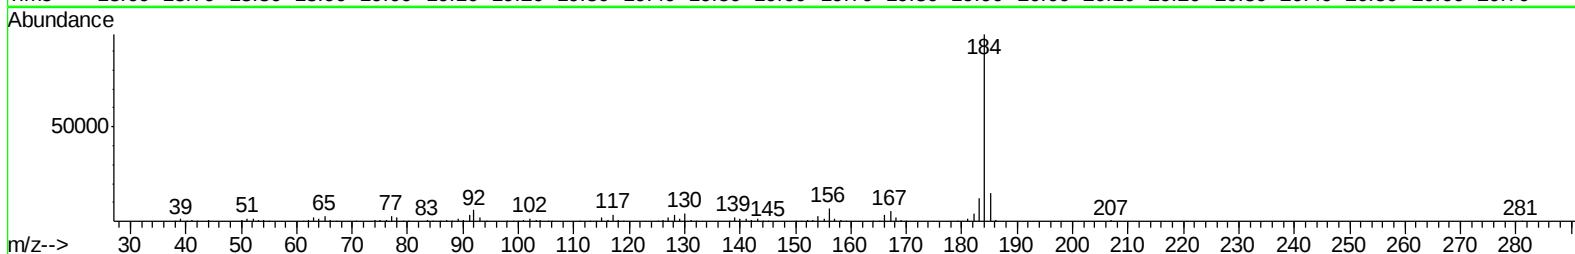


Data Path : Z:\HPCHEM1\BNA G\Data\BG101015\
Data File : BG019113.D
Acq On : 10 Oct 2015 12:23
Operator : UM/NP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 08:07:48 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 12 07:23:23 2015
Response via : Initial Calibration

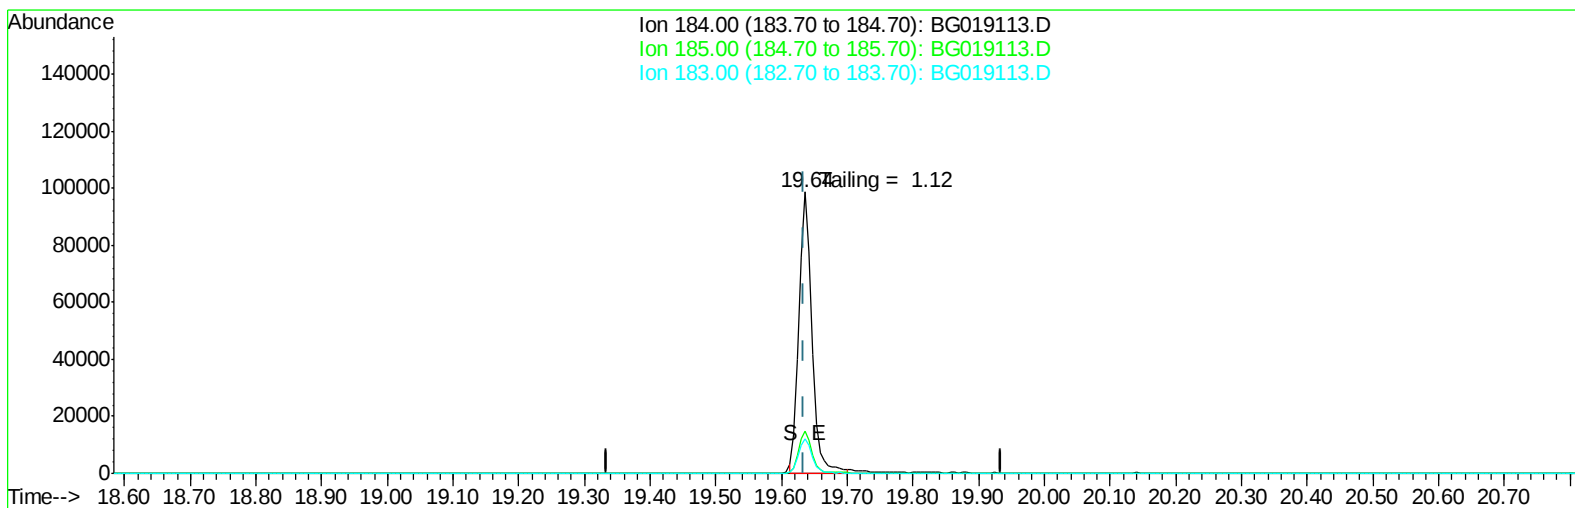

TIC: BG019113.D

(76) Benzidine




19.635min (+0.000) 0.00ng

response 142141

Ion	Exp%	Act%
184.00	100	100
185.00	14.90	15.11
183.00	12.60	12.31
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG101015\
Data File : BG019113.D
Acq On : 10 Oct 2015 12:23
Operator : UM/NP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 08:07:48 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 12 07:23:23 2015
Response via : Initial Calibration

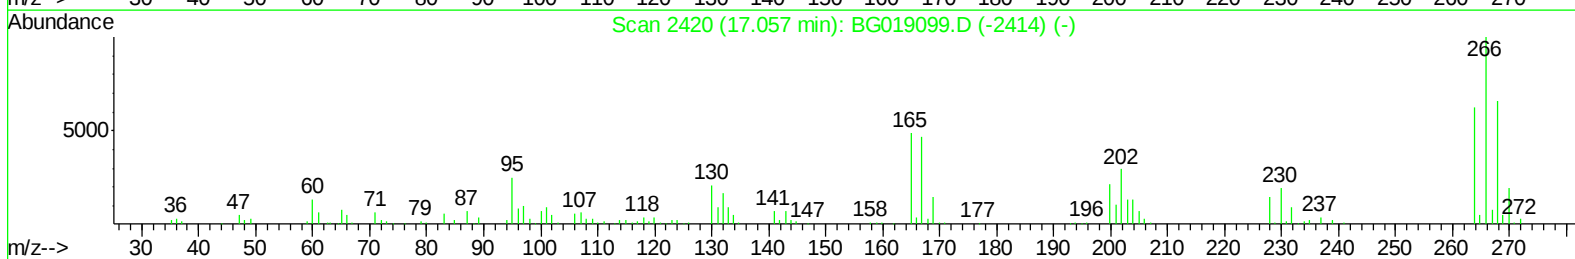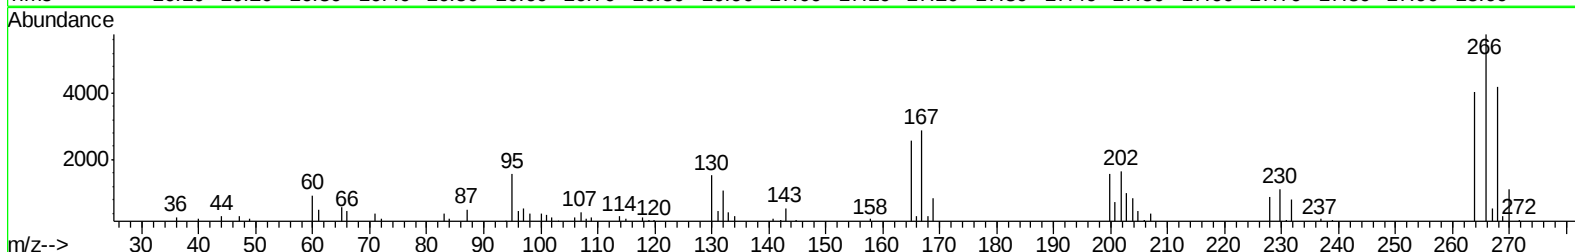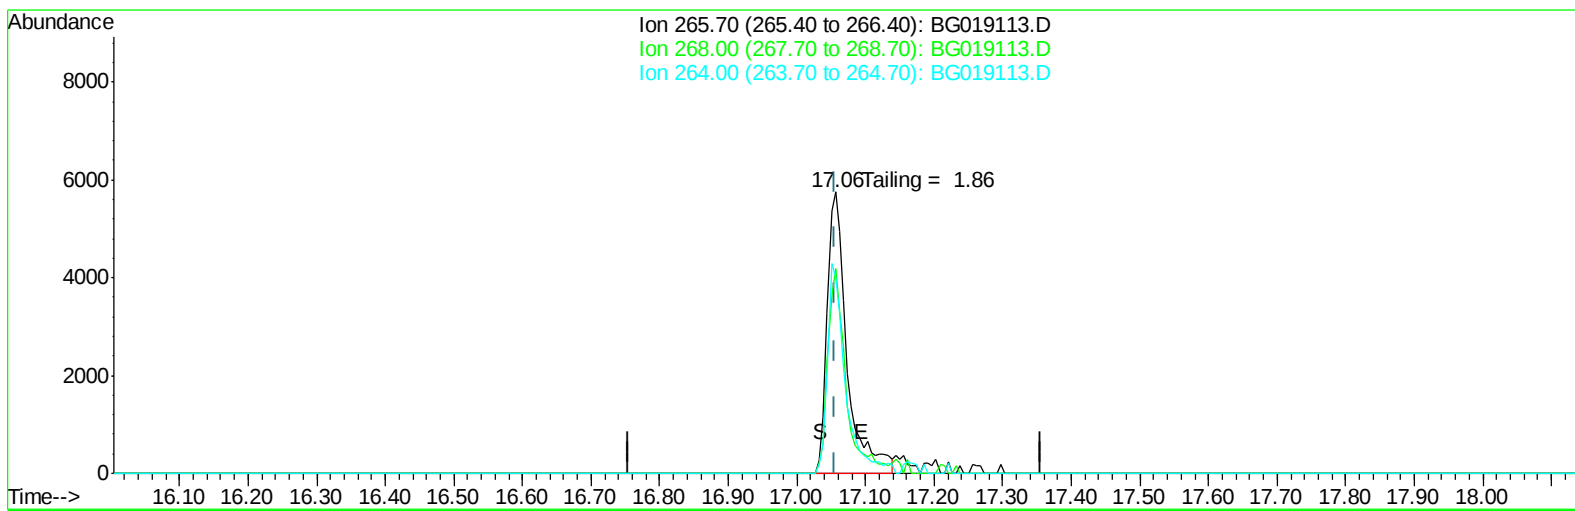

TIC: BG019113.D

(69) Pentachlorophenol (C)

17.056min (+0.000) 0.00ng m

response 11530

Ion	Exp%	Act%
265.70	100	100
268.00	66.20	72.93
264.00	62.60	69.72
0.00	0.00	0.00