
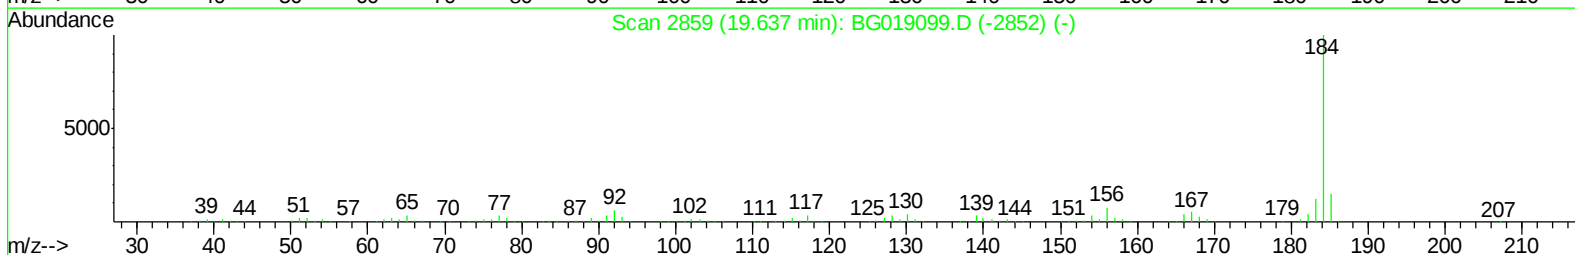
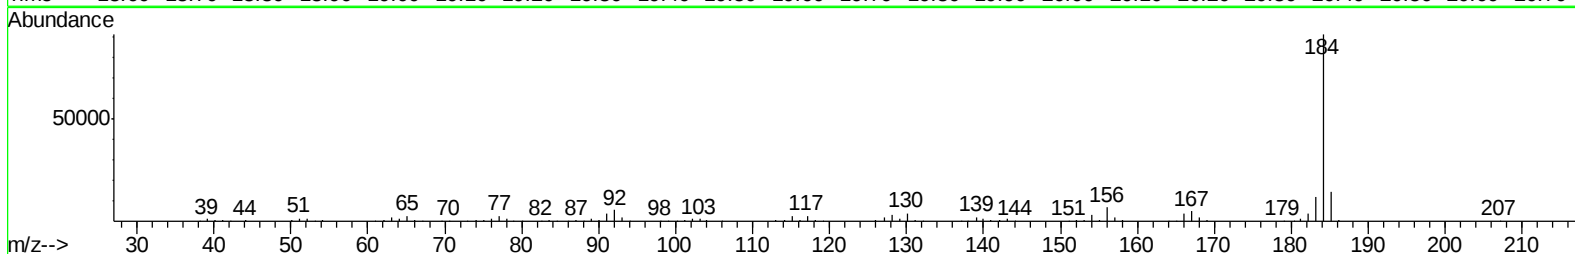


Data Path : Z:\HPCHEM1\BNA G\Data\BG101015\
 Data File : BG019131.D
 Acq On : 10 Oct 2015 23:46
 Operator : UM/NP
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 08:08:50 2015
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101015.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 12 07:23:23 2015
 Response via : Initial Calibration

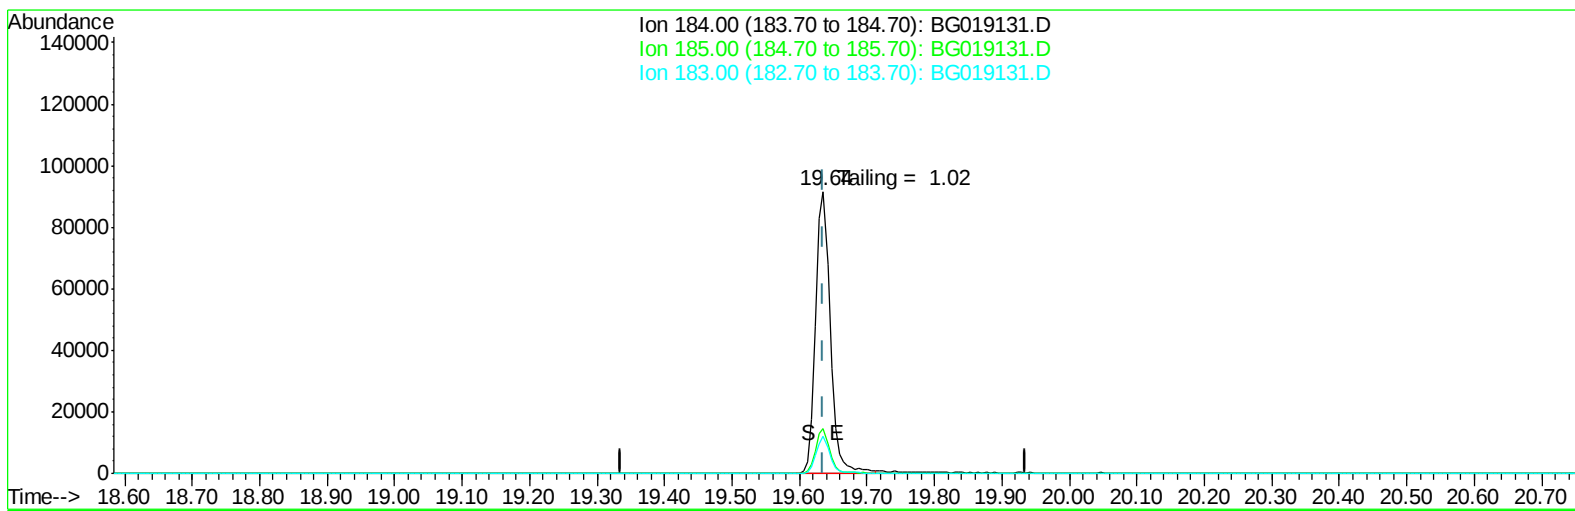

TIC: BG019131.D

(76) Benzidine




19.636min (+0.001) 0.00ng

response 136580

Ion	Exp%	Act%
184.00	100	100
185.00	14.90	16.00
183.00	12.60	13.14
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA G\Data\BG101015\
Data File : BG019131.D
Acq On : 10 Oct 2015 23:46
Operator : UM/NP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 12 08:08:50 2015
Quant Method : Z:\HPCHEM1\BNA G\METHODS\8270-BG101015.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 12 07:23:23 2015
Response via : Initial Calibration

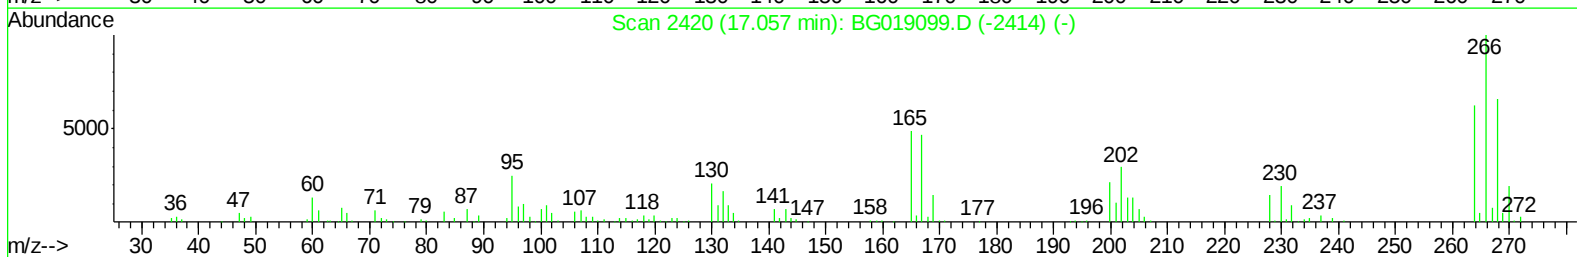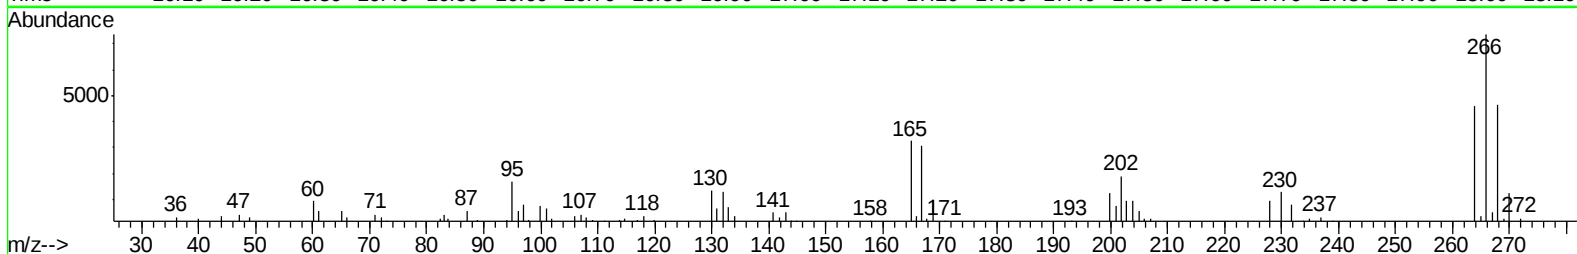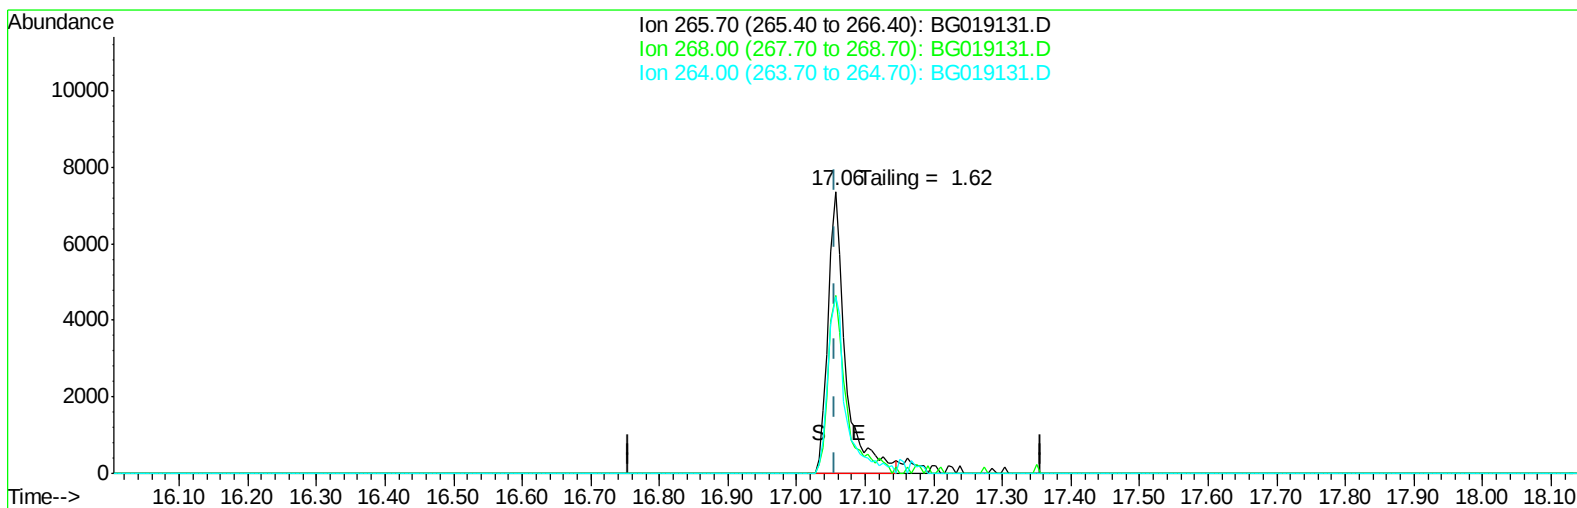

TIC: BG019131.D

(69) Pentachlorophenol (C)

17.056min (+0.001) 0.00ng

response 12860

Ion	Exp%	Act%
265.70	100	100
268.00	66.20	63.24
264.00	62.60	62.62
0.00	0.00	0.00