


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG101015\
Data File : BG019095.D
Acq On : 10 Oct 2015 1:01
Operator : UM/NP
Sample : DFTPP
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG101015.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Oct 10 07:04:31 2015

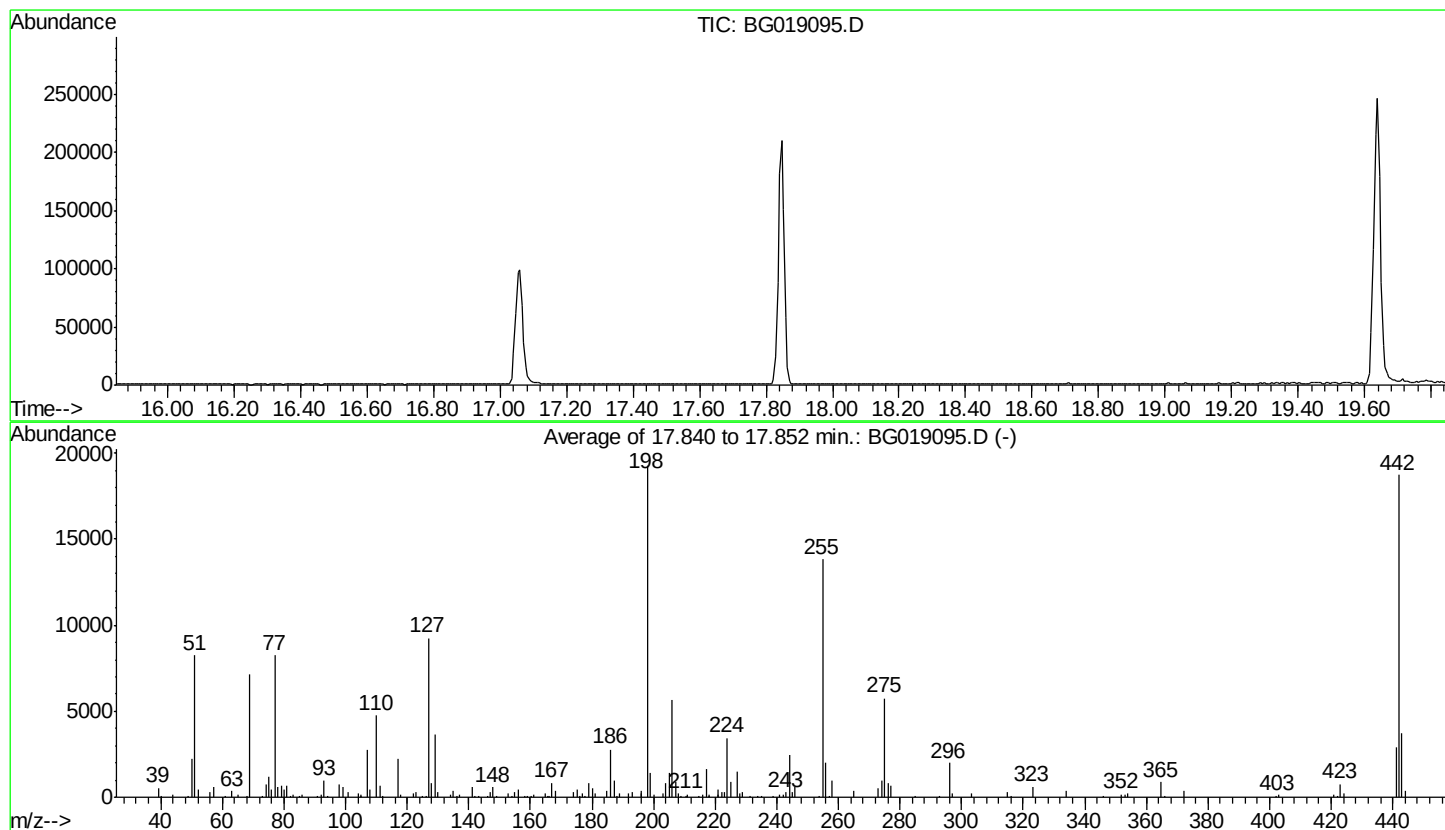

AutoFind: Scans 2553, 2554, 2555; Background Corrected with Scan 2547

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.8	8245	PASS
68	69	0.00	2	1.1	76	PASS
69	198	0.00	100	37.1	7152	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.9	9242	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	19280	PASS
199	198	5	9	7.2	1390	PASS
275	198	10	60	29.8	5751	PASS
365	198	1	100	4.6	879	PASS
441	442	0.01	24	15.6	2925	PASS
442	198	50	100	97.2	18733	PASS
443	442	15	24	19.7	3694	PASS