


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG101015\
Data File : BG019113.D
Acq On : 10 Oct 2015 12:23
Operator : UM/NP
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG101015.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Oct 10 07:04:31 2015

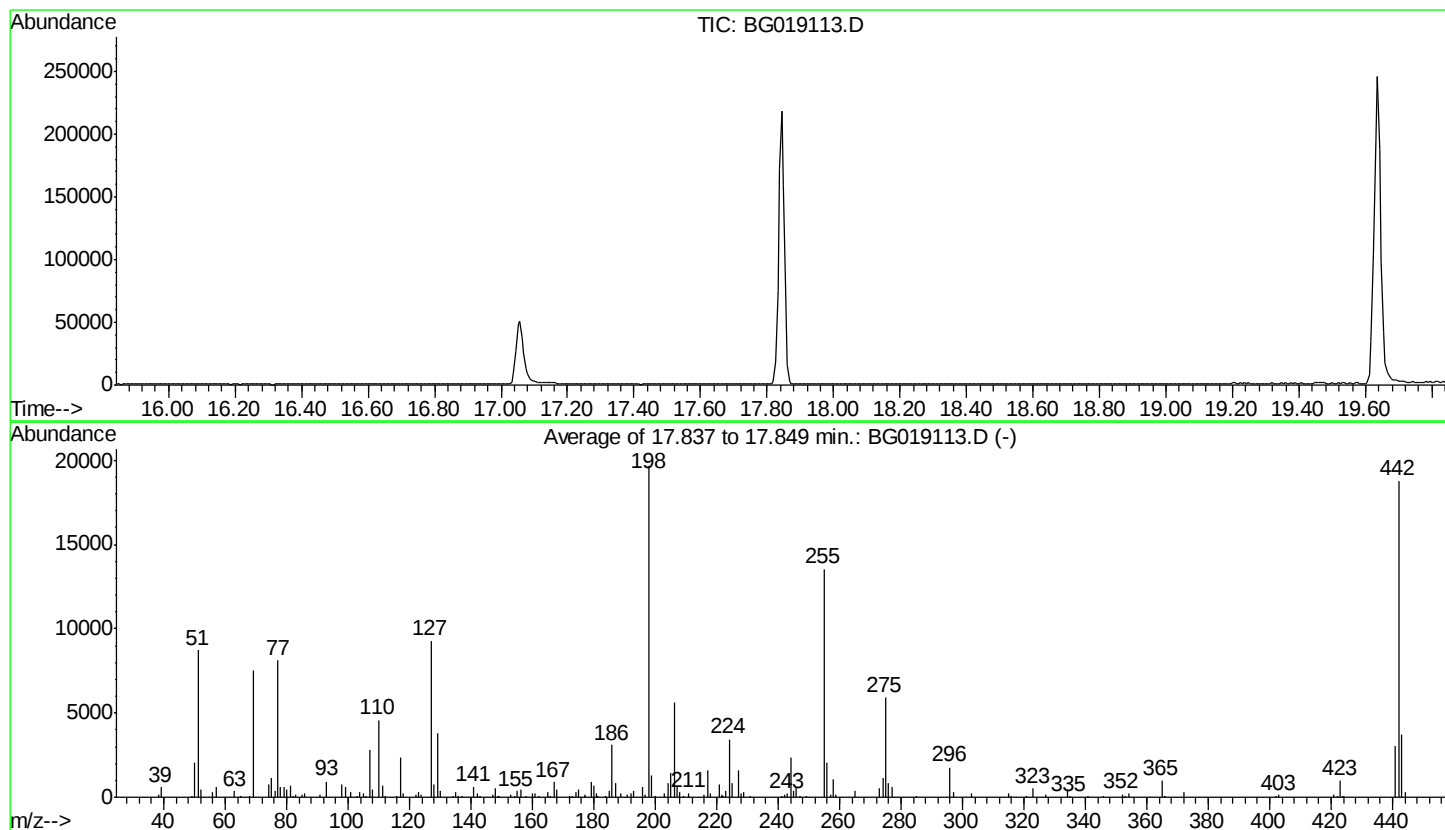

AutoFind: Scans 2553, 2554, 2555; Background Corrected with Scan 2547

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	44.4	8732	PASS
68	69	0.00	2	0.8	57	PASS
69	198	0.00	100	38.2	7506	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.2	9285	PASS
197	198	0.00	2	0.7	144	PASS
198	198	100	100	100.0	19672	PASS
199	198	5	9	6.6	1300	PASS
275	198	10	60	30.0	5899	PASS
365	198	1	100	4.9	973	PASS
441	442	0.01	24	16.3	3064	PASS
442	198	50	100	95.4	18772	PASS
443	442	15	24	19.8	3722	PASS