


Data Path : Z:\HPCHEM1\BNA_G\DATA\BG101015\
 Data File : BG019131.D
 Acq On : 10 Oct 2015 23:46
 Operator : UM/NP
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_G\METHODS\8270-BG101015.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Oct 10 07:04:31 2015

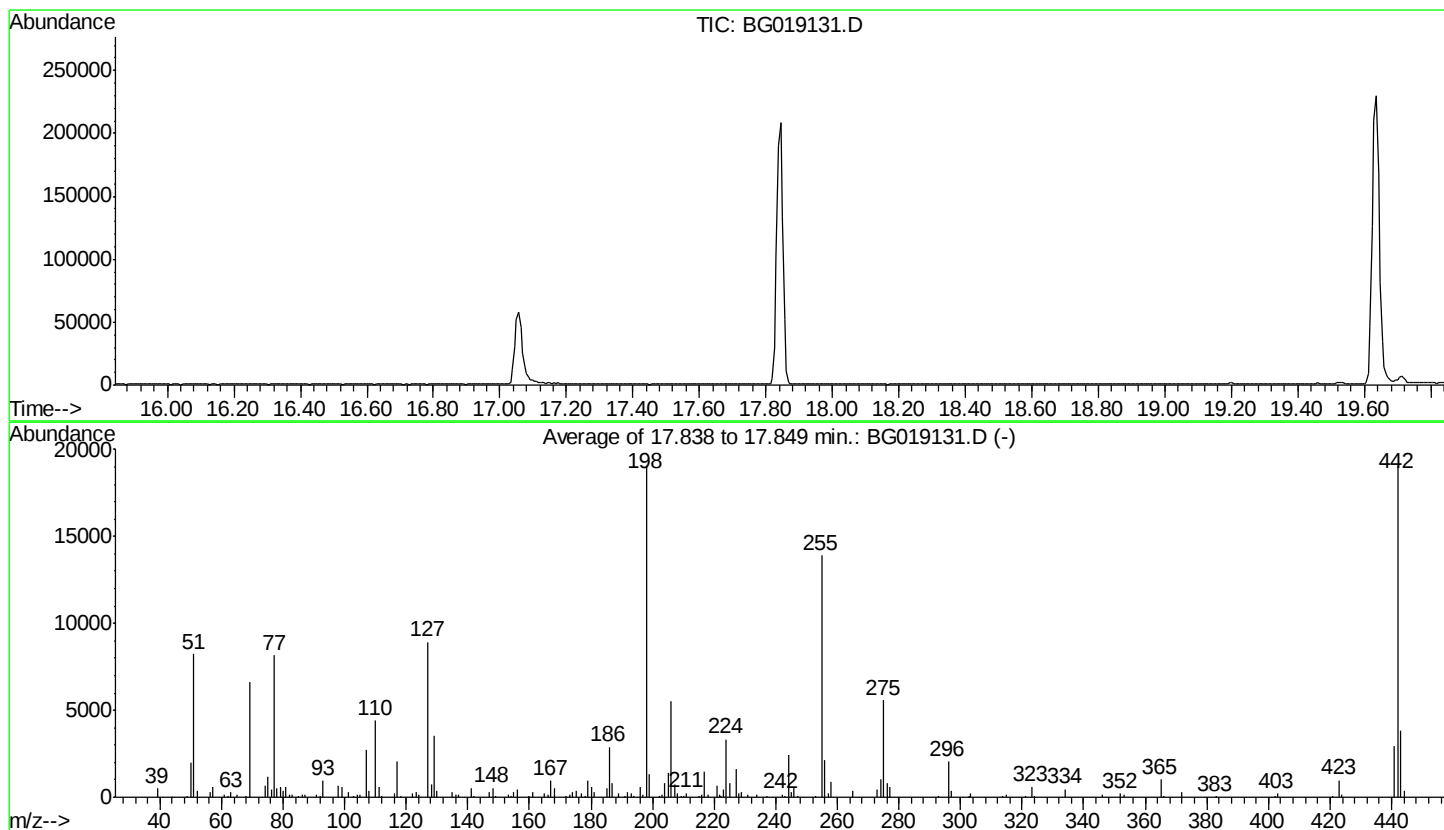

AutoFind: Scans 2553, 2554, 2555; Background Corrected with Scan 2547

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.2	8236	PASS
68	69	0.00	2	1.1	72	PASS
69	198	0.00	100	34.8	6633	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.8	8925	PASS
197	198	0.00	2	0.8	161	PASS
198	198	100	100	100.0	19074	PASS
199	198	5	9	7.0	1328	PASS
275	198	10	60	29.2	5562	PASS
365	198	1	100	5.4	1024	PASS
441	442	0.01	24	15.4	2943	PASS
442	198	50	100	100.0	19070	PASS
443	442	15	24	20.3	3865	PASS