

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101016\
 Data File : BG024239.D
 Acq On : 10 Oct 2016 14:40
 Operator : UM/SJ
 Sample : H5080-11
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDNA9

Manual Integrations
 APPROVED

sohil
 10/11/2016 7:05:14 PM

Quant Time: Oct 10 15:38:45 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Oct 10 13:36:36 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.30	152	120832	20.00	ng/ul	0.00
18) Naphthalene-d8	11.13	136	567919	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.91	164	468859	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.65	188	1026249m	20.00	ng/ul	0.00
75) Chrysene-d12	21.95	240	1134741	20.00	ng/ul	0.00
83) Perylene-d12	25.40	264	1149237	20.00	ng/ul	0.00

System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.65	96	15253	5.99	ng/uL	0.00
5) Phenol-d5	7.43	99	335125	29.73	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.61	67	226768	29.75	ng/ul	0.00
9) 2-Chlorophenol-d4	7.82	132	239455	30.85	ng/ul	0.00
13) 4-Methylphenol-d8	8.98	113	290551	31.88	ng/ul	0.00
19) Nitrobenzene-d5	9.47	128	123066	30.53	ng/ul	0.00
22) 2-Nitrophenol-d4	10.20	143	143992	31.93	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.73	165	273708	27.87	ng/ul	0.00
29) 4-Chloroaniline-d4	11.25	131	366567	35.53	ng/ul	0.00
43) Dimethylphthalate-d6	14.31	166	1035836	31.64	ng/ul	0.00
46) Acenaphthylene-d8	14.61	160	1161984	30.99	ng/ul	0.00
51) 4-Nitrophenol-d4	15.07	143	170945	29.45	ng/ul	0.00
57) Fluorene-d10	15.90	176	973727	31.46	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.00	200	179041m	29.03	ng/ul	0.00
70) Anthracene-d10	17.75	188	1526543	32.93	ng/ul	0.00
76) Pyrene-d10	20.02	212	1756896	33.17	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.17	264	1778783	34.40	ng/ul	0.00

Target Compounds						Ovalue
6) Phenol	7.45	94	12754	1.11	ng/ul#	53
44) Dimethylphthalate	14.35	163	781834	24.36	ng/ul	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA G\DATA\BG101016\
Data File : BG024239.D
Acq On : 10 Oct 2016 14:40
Operator : UM/SJ
Sample : H5080-11
Misc :
ALS Vial : 6 Sample Multiplier: 1


Instrument :
BNA_G
ClientSampleId :
BDNA9

Manual Integrations
APPROVED

sohil
10/11/2016 7:05:14 PM

Quant Time: Oct 10 15:38:45 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Oct 10 13:36:36 2016
Response via : Initial Calibration

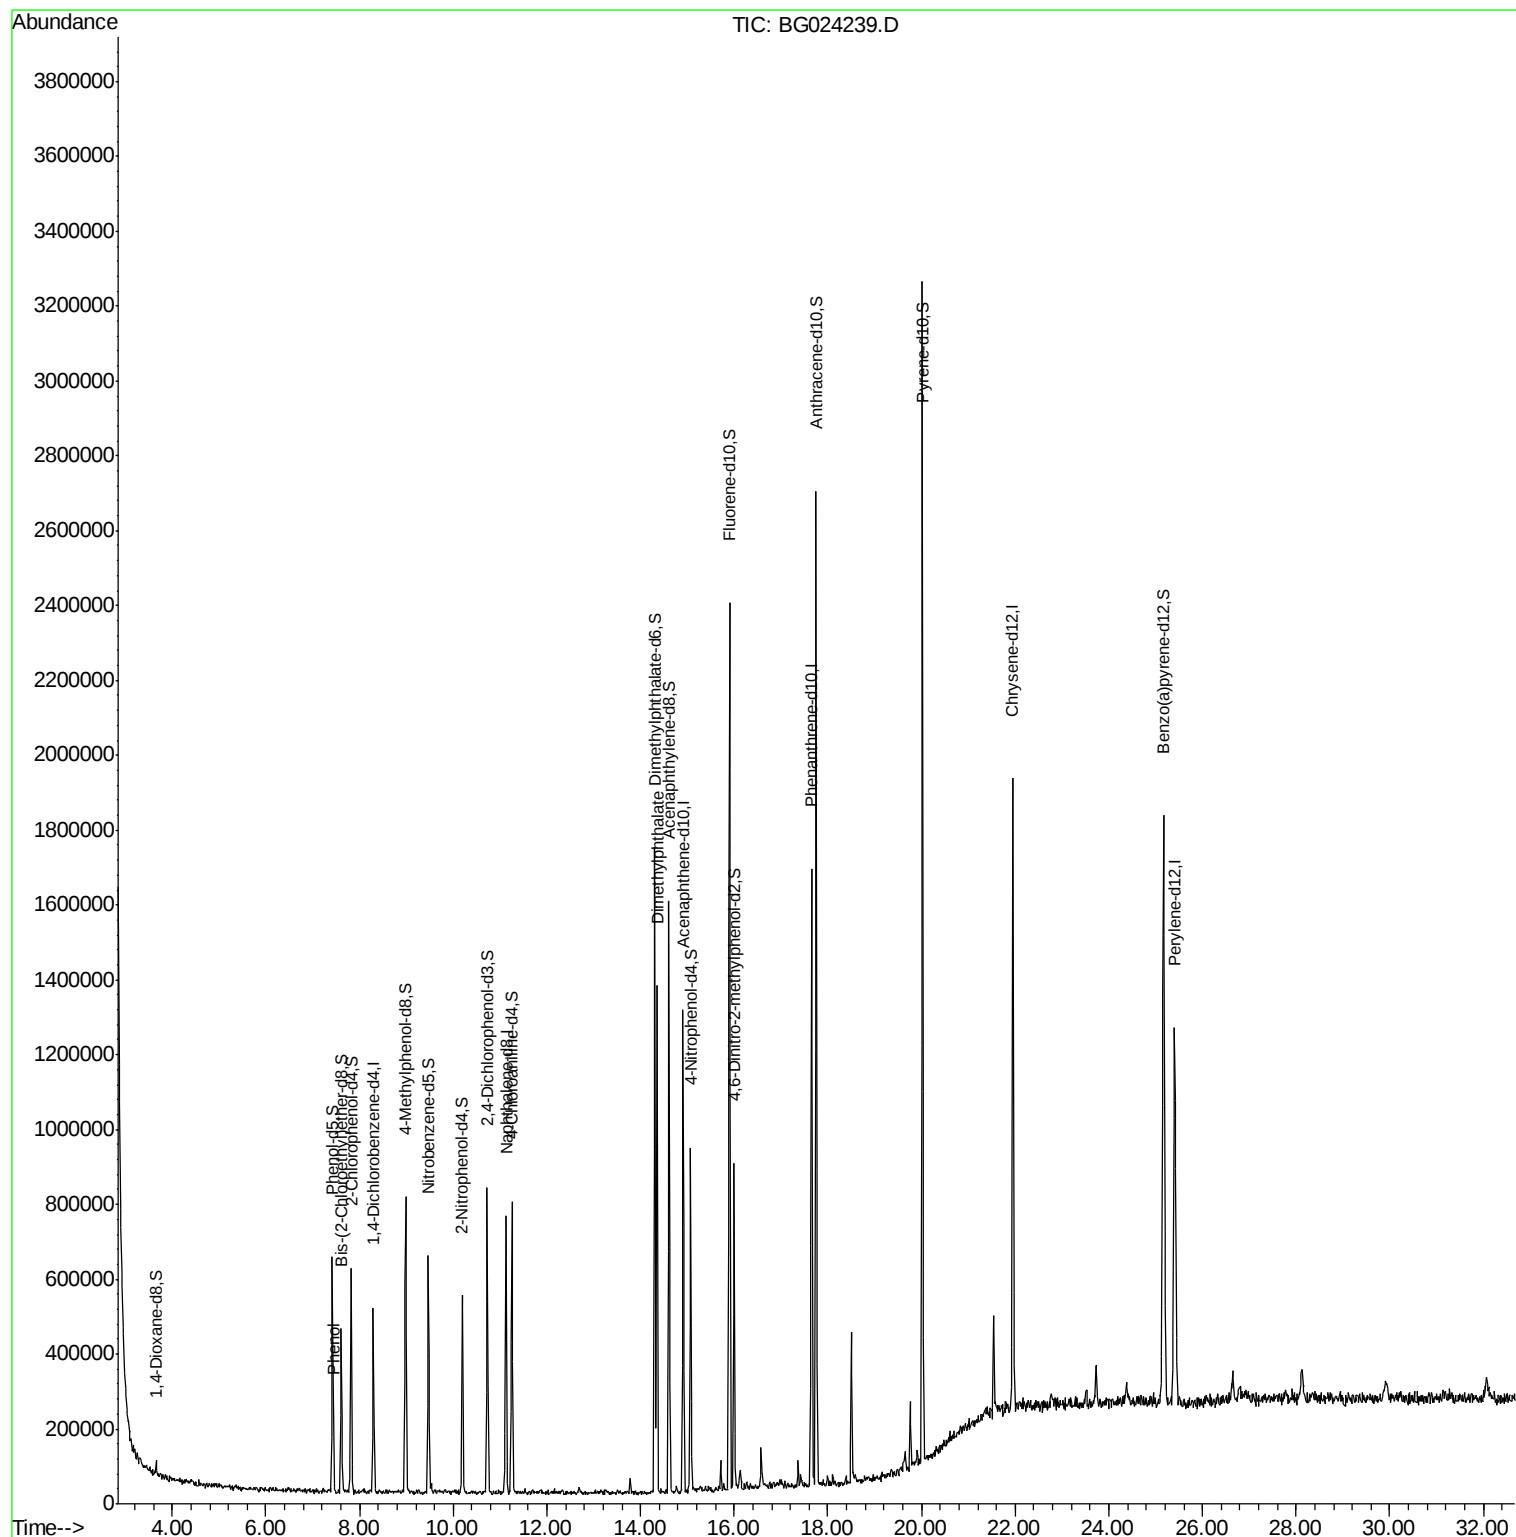

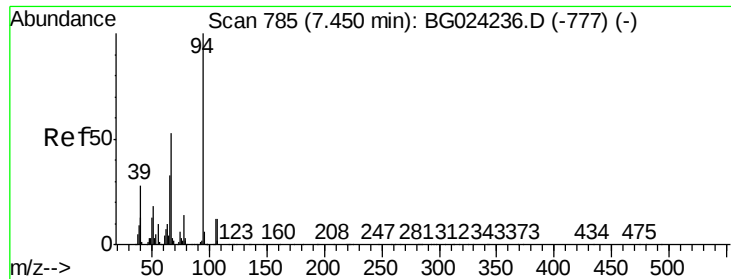

#6

Phenol

Concen: 1.11 ng/ul

RT: 7.45 min Scan# 785

Delta R.T. -0.00 min

Lab File: BG024239.D

Acq: 10 Oct 2016 14:40

Instrument :

BNA_G





ClientSampled :

BDNA9

Tot Ion:	94	Resp:	12754
Ion Ratio	Lower	Upper	
94	100		
65	35.6	16.8	25.2#
66	58.8	22.6	33.8#

Manual Integrations
APPROVED

sohil
10/11/2016 7:05:14 PM

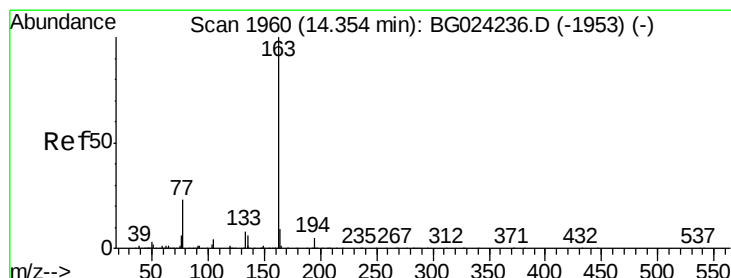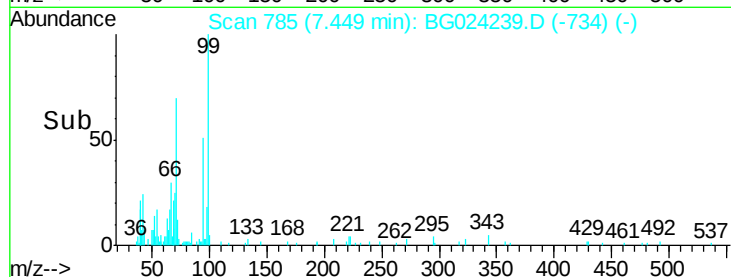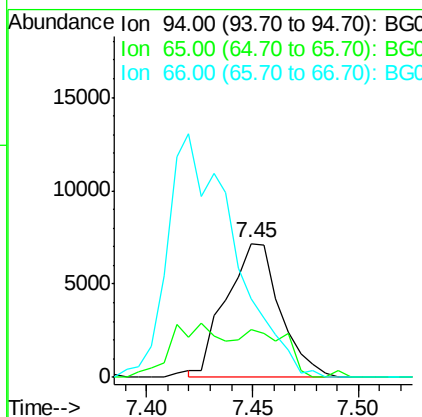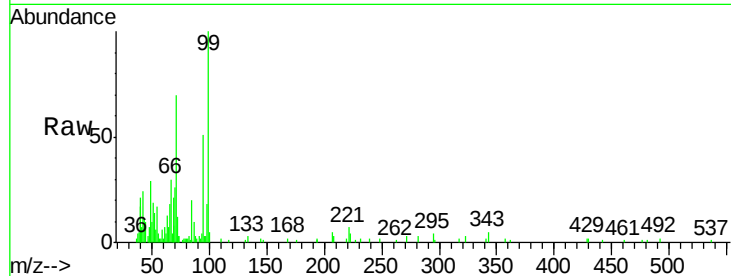

#44

Dimethylphthalate

Concen: 24.36 ng/ul

RT: 14.35 min Scan# 1960

Delta R.T. -0.00 min

Lab File: BG024239.D

Acq: 10 Oct 2016 14:40

Tgt Ion:	163	Resp:	781834
Ion Ratio	Lower	Upper	
163	100		
194	4.7	3.4	5.2
164	10.0	8.8	13.2

