

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101016\
 Data File : BG024248.D
 Acq On : 10 Oct 2016 21:06
 Operator : UM/SJ
 Sample : H5098-05
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDNF1

Quant Time: Oct 11 10:32:39 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 11 10:18:36 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.29	152	161340	20.00	ng/ul	-0.01
18) Naphthalene-d8	11.13	136	695198	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.91	164	566333	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.65	188	1193091	20.00	ng/ul	0.00
75) Chrysene-d12	21.95	240	1311412	20.00	ng/ul	0.00
83) Perylene-d12	25.40	264	1339425	20.00	ng/ul	-0.01

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.65	96	11071	3.26	ng/uL	0.00
5) Phenol-d5	7.42	99	291521	19.37	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.61	67	202344	19.88	ng/ul	0.00
9) 2-Chlorophenol-d4	7.81	132	204184	19.70	ng/ul	0.00
13) 4-Methylphenol-d8	8.98	113	224549	18.45	ng/ul	0.00
19) Nitrobenzene-d5	9.47	128	108911	22.08	ng/ul	0.00
22) 2-Nitrophenol-d4	10.19	143	126229	22.87	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.73	165	233535	19.43	ng/ul	0.00
29) 4-Chloroaniline-d4	11.25	131	256437	20.30	ng/ul	0.00
43) Dimethylphthalate-d6	14.31	166	853424	21.58	ng/ul	0.00
46) Acenaphthylene-d8	14.61	160	1002596	22.13	ng/ul	0.00
51) 4-Nitrophenol-d4	15.07	143	135359	19.31	ng/ul	0.00
57) Fluorene-d10	15.89	176	816919	21.85	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.99	200	142305	19.85	ng/ul	0.00
70) Anthracene-d10	17.75	188	1241072	23.03	ng/ul	0.00
76) Pyrene-d10	20.02	212	1406931	22.99	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.16	264	1360271	22.57	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.35	163	549662	14.18	ng/ul	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101016\
Data File : BG024248.D
Acq On : 10 Oct 2016 21:06
Operator : UM/SJ
Sample : H5098-05
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDNF1

Quant Time: Oct 11 10:32:39 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 11 10:18:36 2016
Response via : Initial Calibration

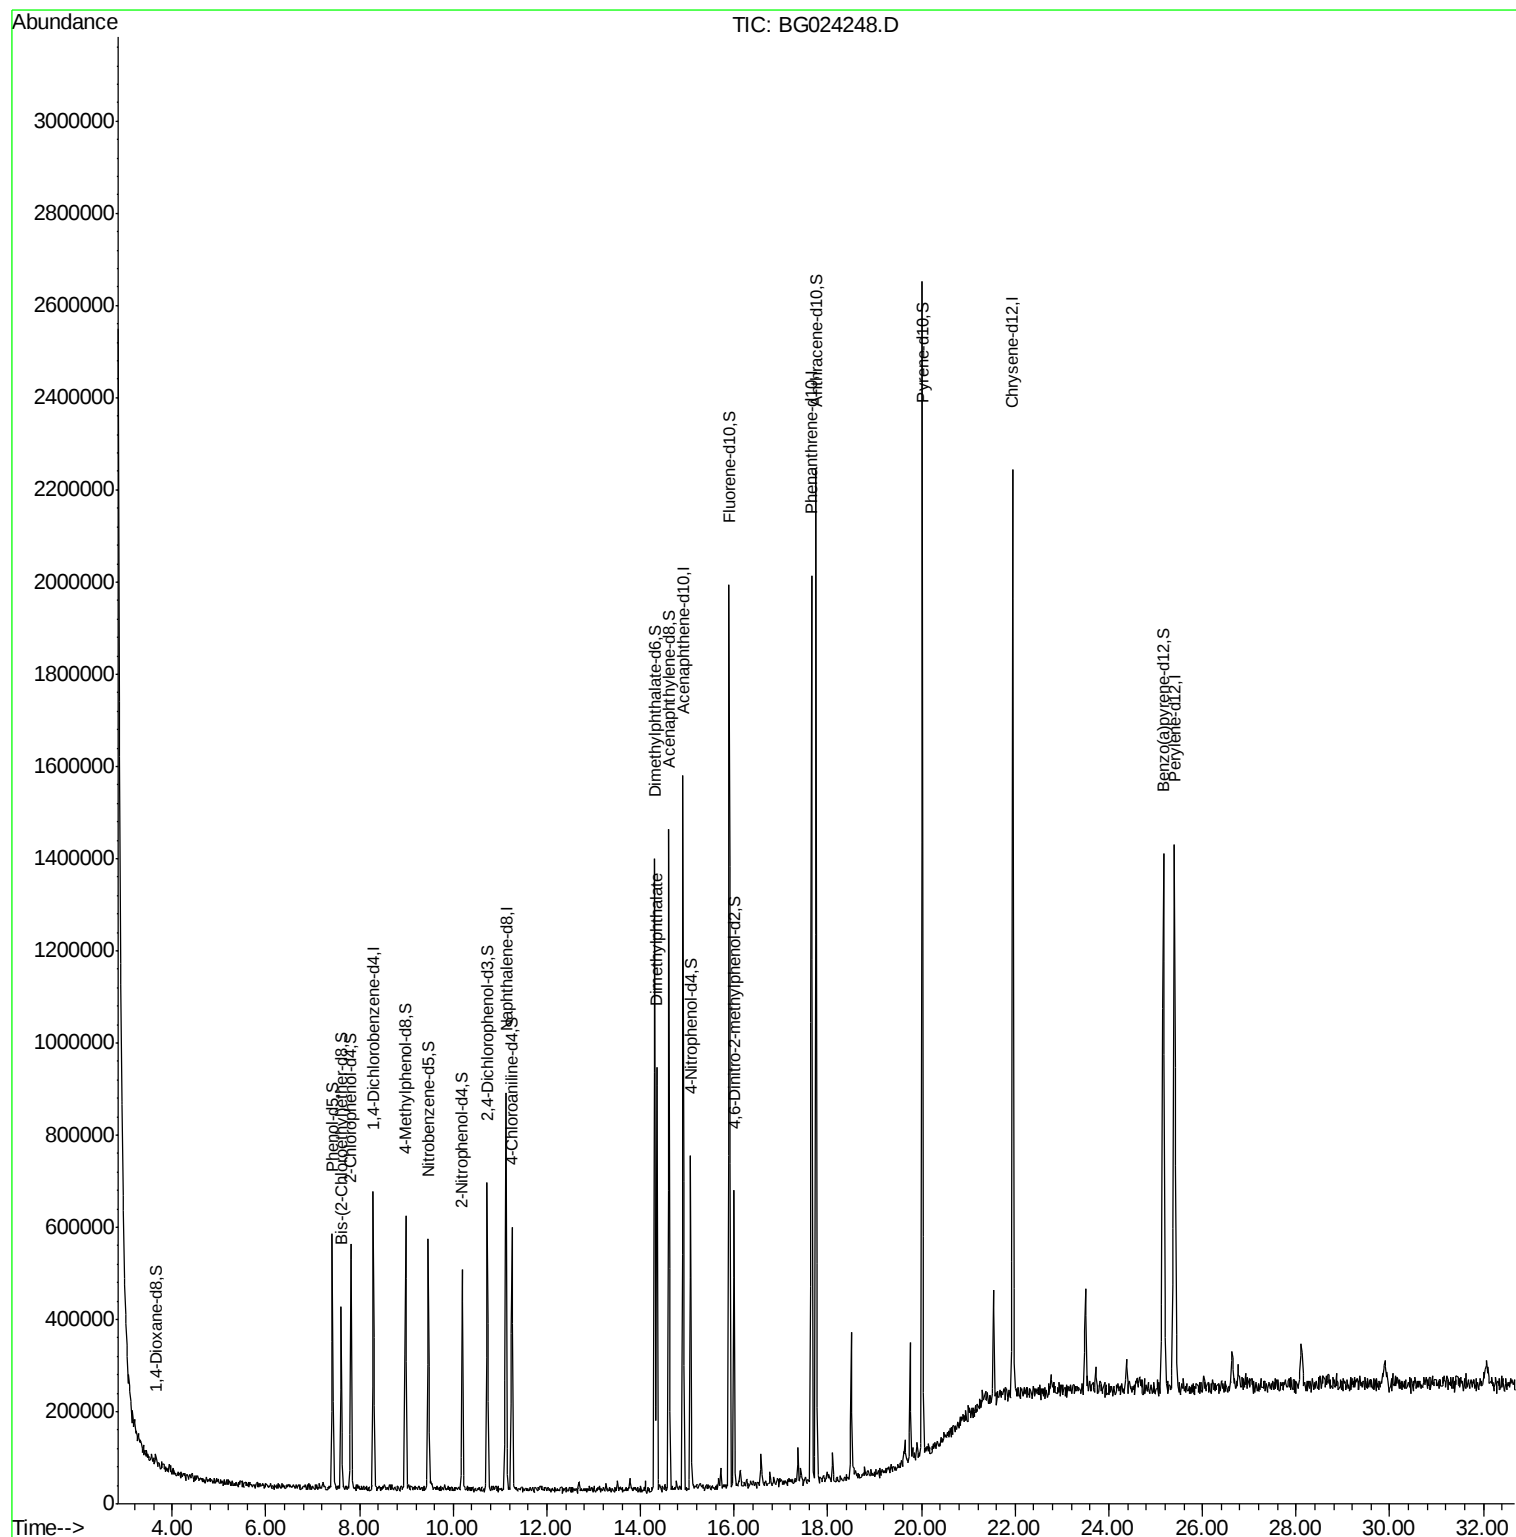

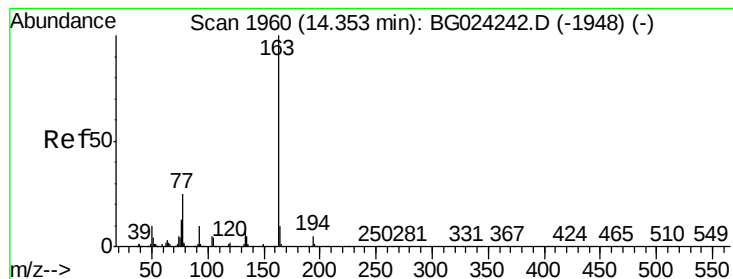

#44
 Dimethylphthalate
 Concen: 14.18 ng/ul
 RT: 14.35 min Scan# 1959
 Delta R.T. -0.01 min
 Lab File: BG024248.D
 Acq: 10 Oct 2016 21:06

Instrument :
 BNA_G
 ClientSampleId :
 BDNF1

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.9	3.4	5.2
164	11.1	8.8	13.2

