

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101016\
 Data File : BG024254.D
 Acq On : 11 Oct 2016 00:56
 Operator : UM/SJ
 Sample : H5098-11
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDNP6

Quant Time: Oct 11 11:25:56 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 11 10:18:36 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.29	152	167686	20.00	ng/ul	-0.01
18) Naphthalene-d8	11.12	136	707254	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.91	164	550581	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.65	188	1147209	20.00	ng/ul	0.00
75) Chrysene-d12	21.95	240	1356850	20.00	ng/ul	0.00
83) Perylene-d12	25.40	264	1391505	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.65	96	17785	5.04	ng/uL	0.00
5) Phenol-d5	7.42	99	377204	24.11	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.61	67	284301	26.88	ng/ul	0.00
9) 2-Chlorophenol-d4	7.82	132	286364	26.58	ng/ul	0.00
13) 4-Methylphenol-d8	8.98	113	272290	21.53	ng/ul	-0.01
19) Nitrobenzene-d5	9.47	128	148726	29.63	ng/ul	0.00
22) 2-Nitrophenol-d4	10.19	143	165400	29.45	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.73	165	317654	25.97	ng/ul	0.00
29) 4-Chloroaniline-d4	11.25	131	387669	30.17	ng/ul	0.00
43) Dimethylphthalate-d6	14.31	166	1103285	28.70	ng/ul	0.00
46) Acenaphthylene-d8	14.61	160	1291115	29.32	ng/ul	0.00
51) 4-Nitrophenol-d4	15.07	143	176821	25.94	ng/ul	0.00
57) Fluorene-d10	15.89	176	1046467	28.79	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.00	200	200863	29.13	ng/ul	0.00
70) Anthracene-d10	17.75	188	1616101	31.19	ng/ul	0.00
76) Pyrene-d10	20.02	212	1874842	29.60	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.16	264	1952887	31.19	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.35	163	626425	16.62	ng/ul#	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101016\
Data File : BG024254.D
Acq On : 11 Oct 2016 00:56
Operator : UM/SJ
Sample : H5098-11
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDNP6

Quant Time: Oct 11 11:25:56 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 11 10:18:36 2016
Response via : Initial Calibration

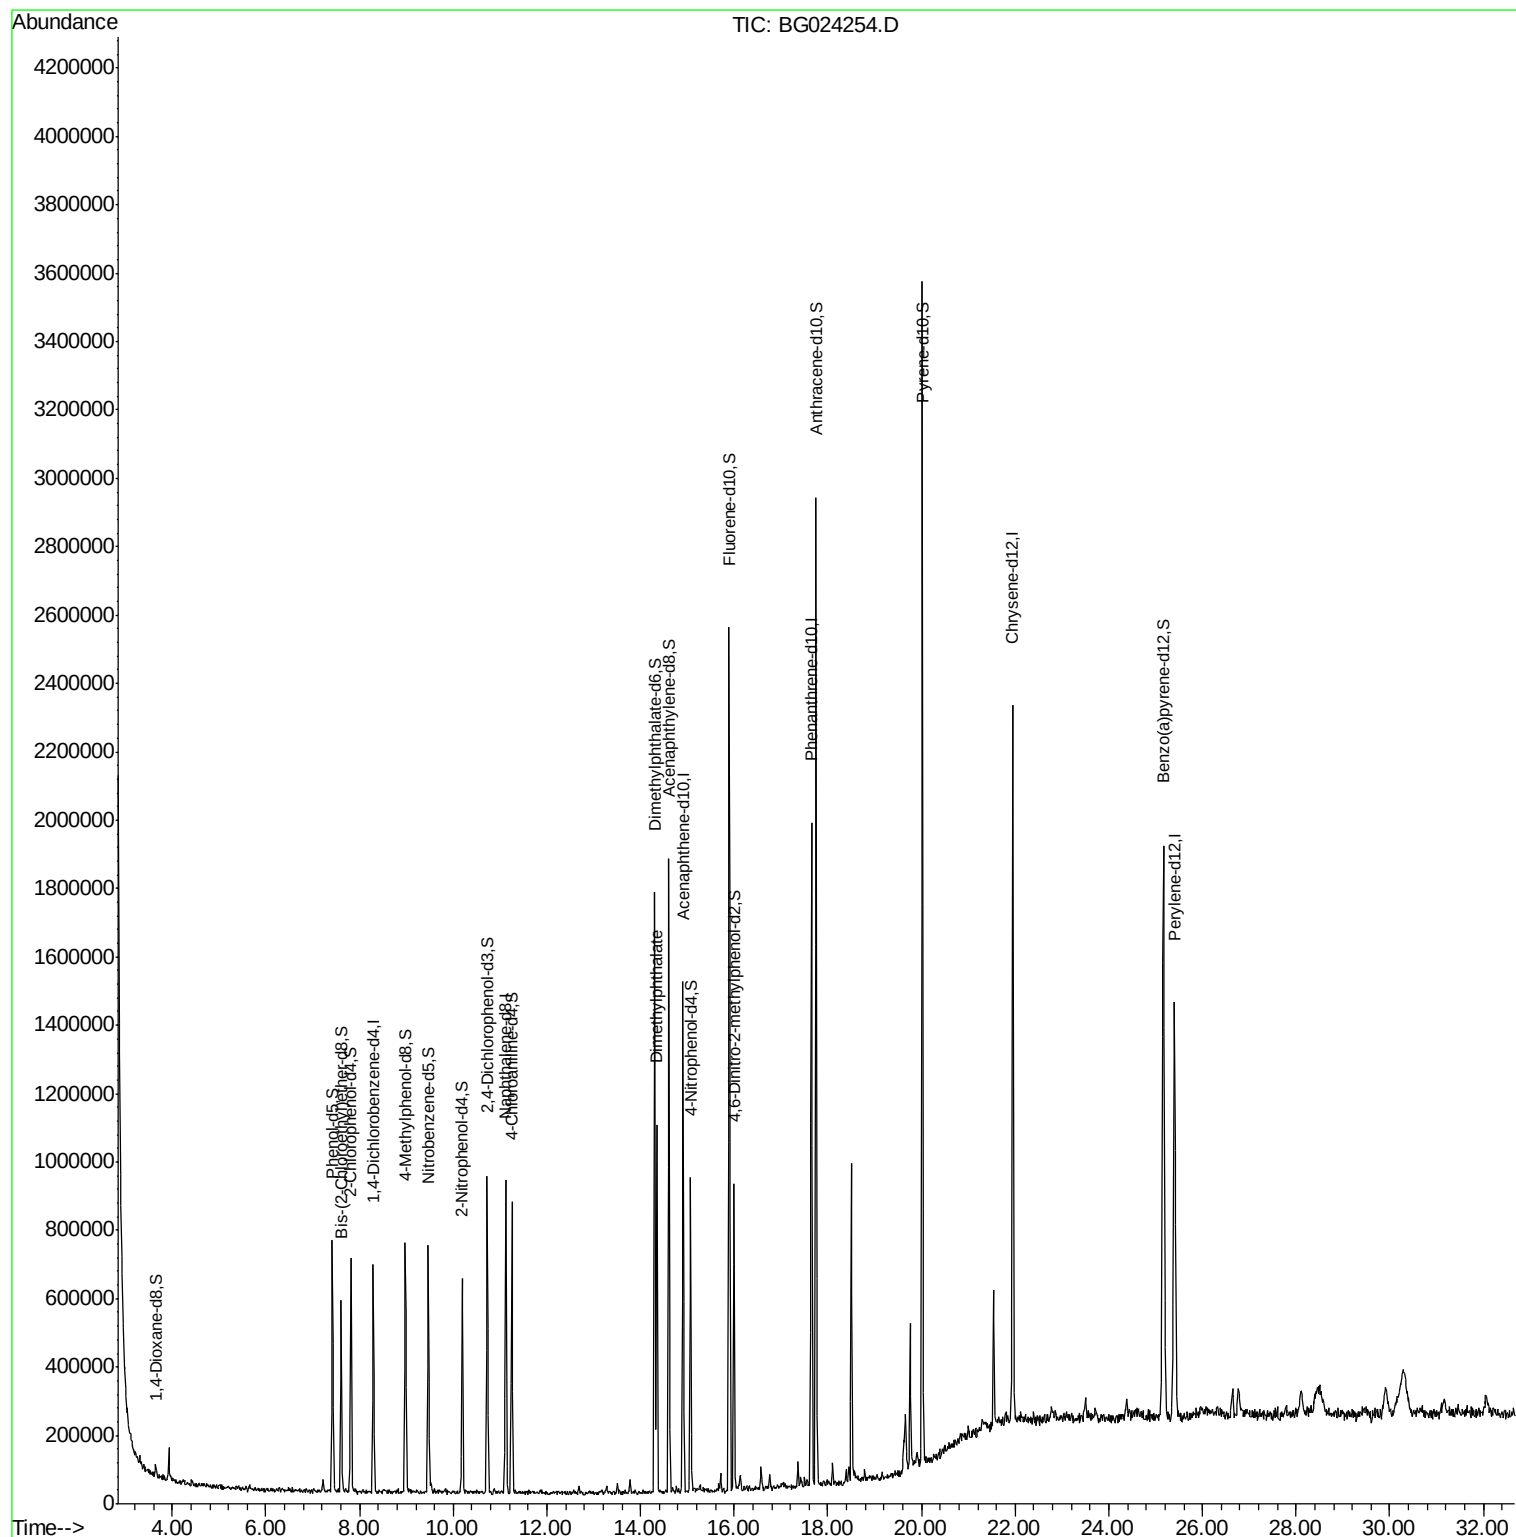

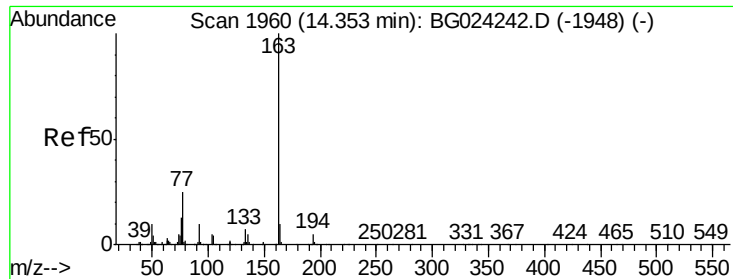

#44

Dimethylphthalate

Concen: 16.62 ng/ul

RT: 14.35 min Scan# 1959

Delta R.T. -0.01 min

Lab File: BG024254.D

Acq: 11 Oct 2016 00:56

Instrument :

BNA_G

ClientSampleId :

BDNP6


Tot Ion:163 Resp: 626425

Ion Ratio Lower Upper

163 100

194 5.4 3.4 5.2#

164 9.9 8.8 13.2

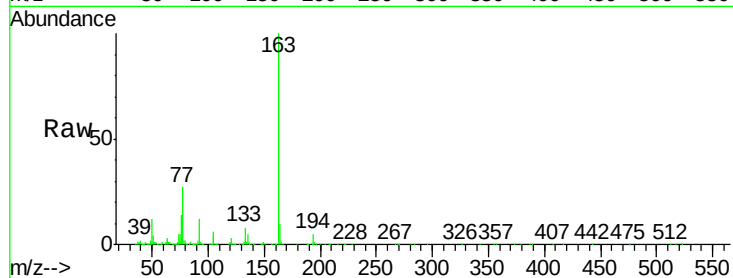

Abundance Ion 163.00 (162.70 to 163.70): E

Ion 194.00 (193.70 to 194.70): E

Ion 164.00 (163.70 to 164.70): E

