

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101016\
 Data File : BG024256.D
 Acq On : 11 Oct 2016 2:13
 Operator : UM/SJ
 Sample : H5098-13
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 BDNG1

Quant Time: Oct 11 11:36:42 2016
 Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Oct 11 10:18:36 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.29	152	170281	20.00	ng/ul	0.00
18) Naphthalene-d8	11.12	136	723063	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.91	164	604756	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.65	188	1266290	20.00	ng/ul	0.00
75) Chrysene-d12	21.95	240	1400270	20.00	ng/ul	0.00
83) Perylene-d12	25.40	264	1417991	20.00	ng/ul	-0.02

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.65	96	6479	1.81	ng/uL	0.00
5) Phenol-d5	7.42	99	144829	9.12	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.61	67	109689	10.21	ng/ul	0.00
9) 2-Chlorophenol-d4	7.82	132	102702	9.39	ng/ul	0.00
13) 4-Methylphenol-d8	8.98	113	93830	7.31	ng/ul	0.00
19) Nitrobenzene-d5	9.46	128	53858	10.50	ng/ul	-0.02
22) 2-Nitrophenol-d4	10.20	143	60060	10.46	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.73	165	118637	9.49	ng/ul	0.00
29) 4-Chloroaniline-d4	11.25	131	139077	10.59	ng/ul	0.00
43) Dimethylphthalate-d6	14.30	166	474081	11.23	ng/ul	0.00
46) Acenaphthylene-d8	14.61	160	530637	10.97	ng/ul	0.00
51) 4-Nitrophenol-d4	15.07	143	78687	10.51	ng/ul	0.00
57) Fluorene-d10	15.90	176	446141	11.18	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	16.00	200	84713	11.13	ng/ul	0.00
70) Anthracene-d10	17.75	188	736535	12.88	ng/ul	0.00
76) Pyrene-d10	20.01	212	983401	15.05	ng/ul	0.00
87) Benzo(a)pyrene-d12	25.16	264	932645	14.62	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Ovalue
44) Dimethylphthalate	14.35	163	314707	7.60	ng/ul	96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA G\DATA\BG101016\
Data File : BG024256.D
Acq On : 11 Oct 2016 2:13
Operator : UM/SJ
Sample : H5098-13
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
BDNG1

Quant Time: Oct 11 11:36:42 2016
Quant Method : Z:\HPCHEM1\BNA G\METHODS\SOM02.2-EPA-BG0100716.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Oct 11 10:18:36 2016
Response via : Initial Calibration

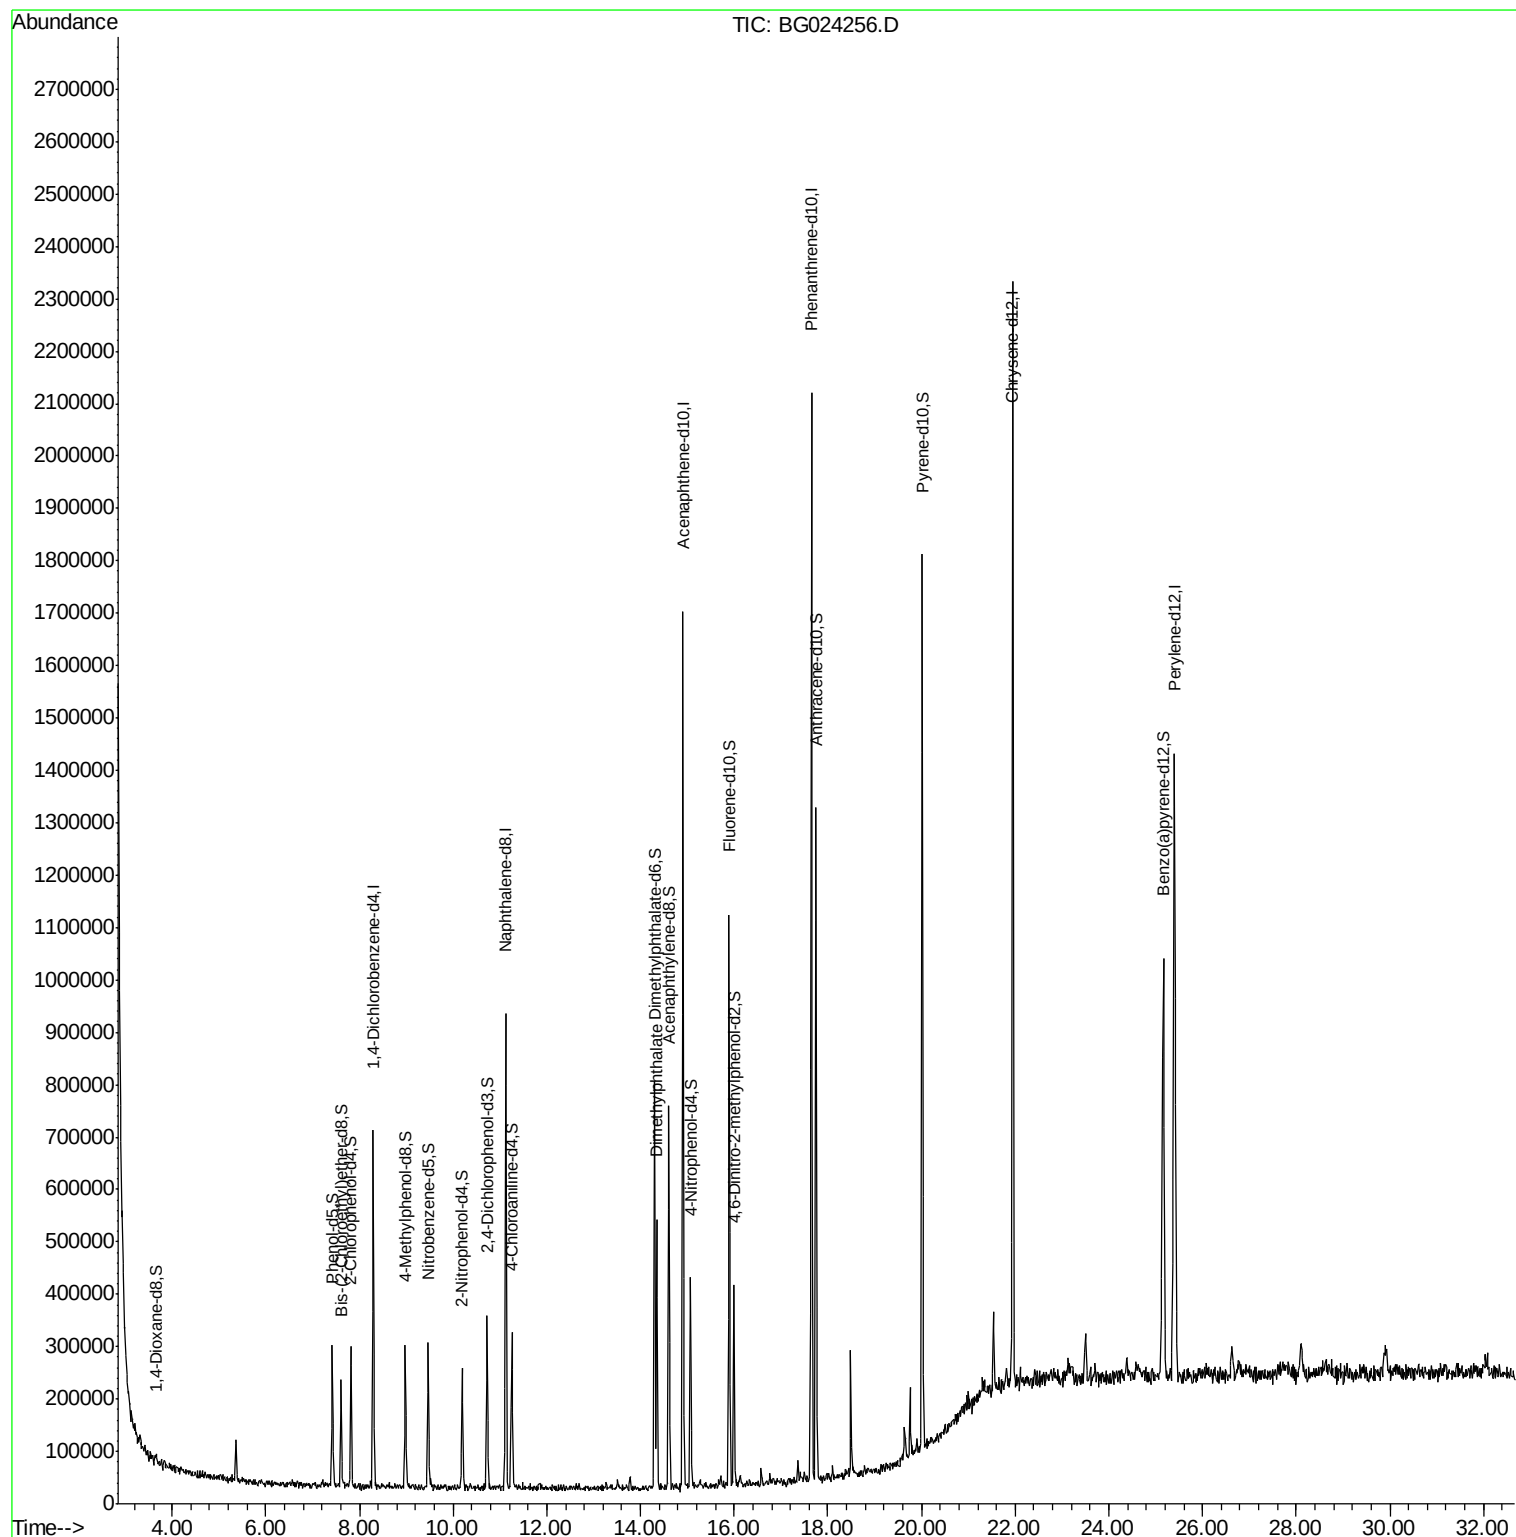

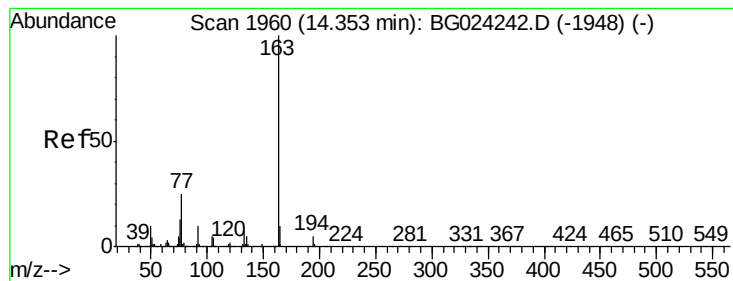

#44

Dimethylphthalate

Concen: 7.60 ng/ul

RT: 14.35 min Scan# 1959

Delta R.T. -0.00 min

Lab File: BG024256.D

Acq: 11 Oct 2016 2:13

Instrument :

BNA_G

ClientSampleId :

BDNG1

Tot Ion:163 Resp: 314707

Ion Ratio Lower Upper

163 100

194 5.0 3.4 5.2

164 9.2 8.8 13.2

