
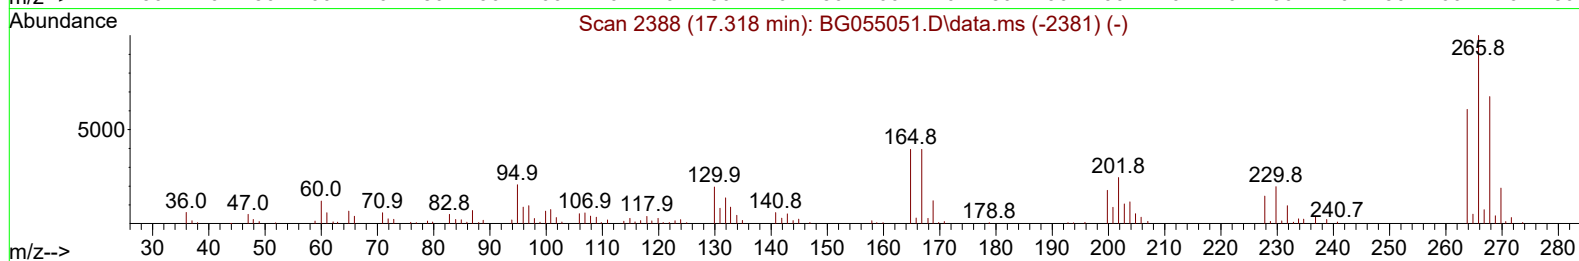
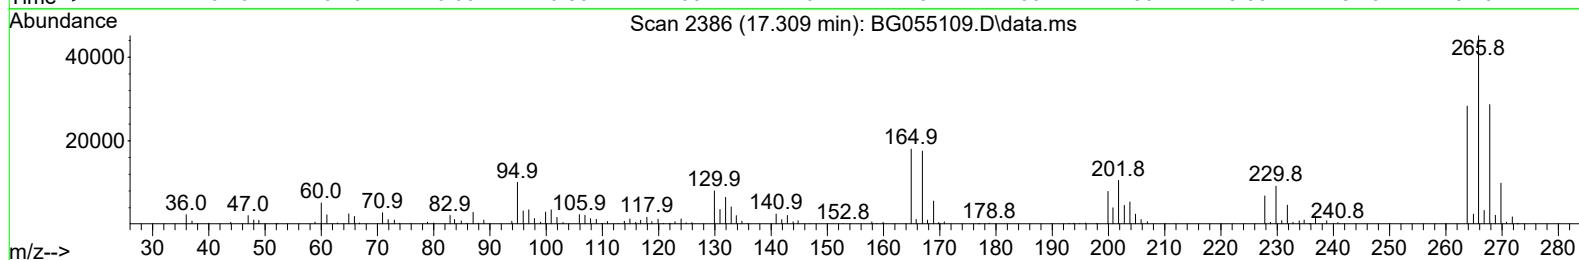


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101022\
Data File : BG055109.D
Acq On : 10 Oct 2022 11:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 11 06:15:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 08 03:04:59 2022
Response via : Initial Calibration

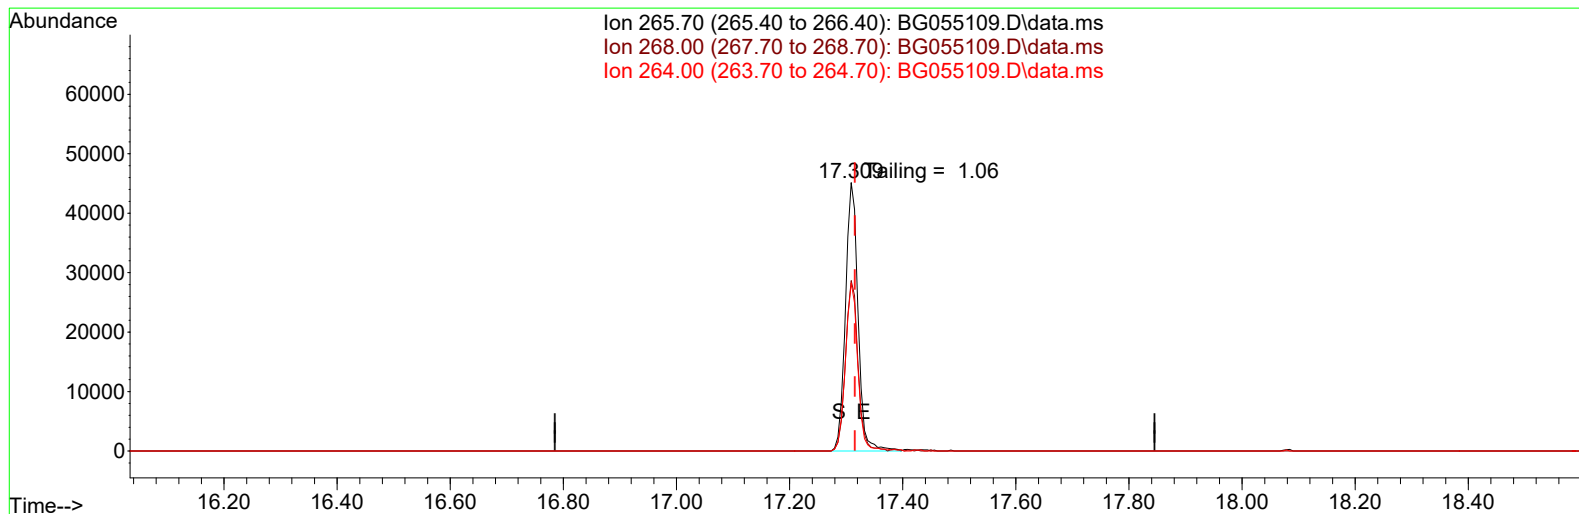

TIC: BG055109.D\data.ms

(70) Pentachlorophenol (C)




17.309min (-0.007) 29399.91 ng

response 69824

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.50	63.53
264.00	60.80	62.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101022\
 Data File : BG055109.D
 Acq On : 10 Oct 2022 11:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 11 06:15:53 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 08 03:04:59 2022
 Response via : Initial Calibration

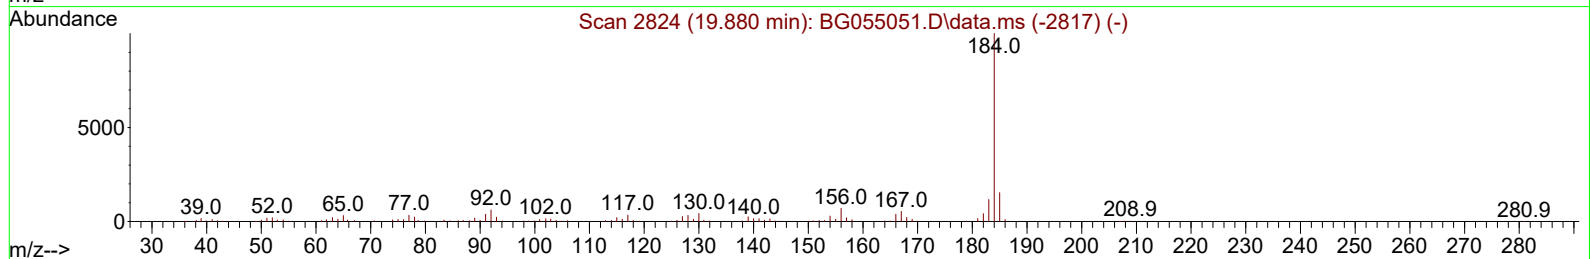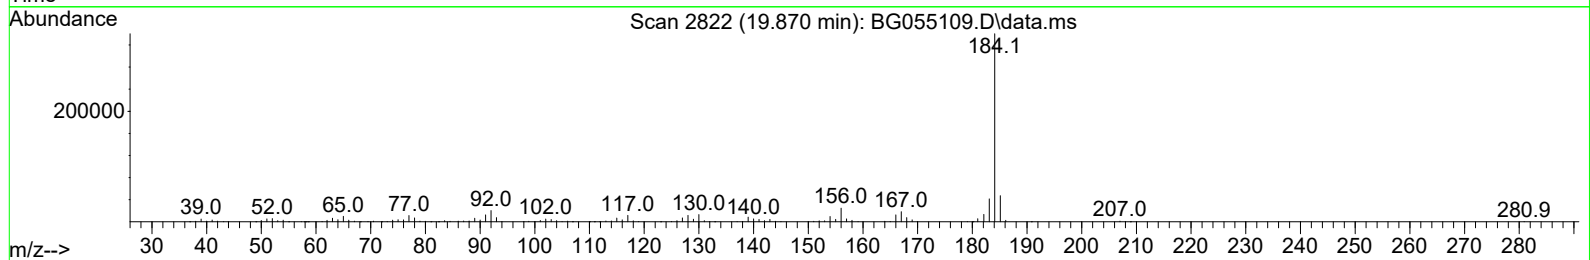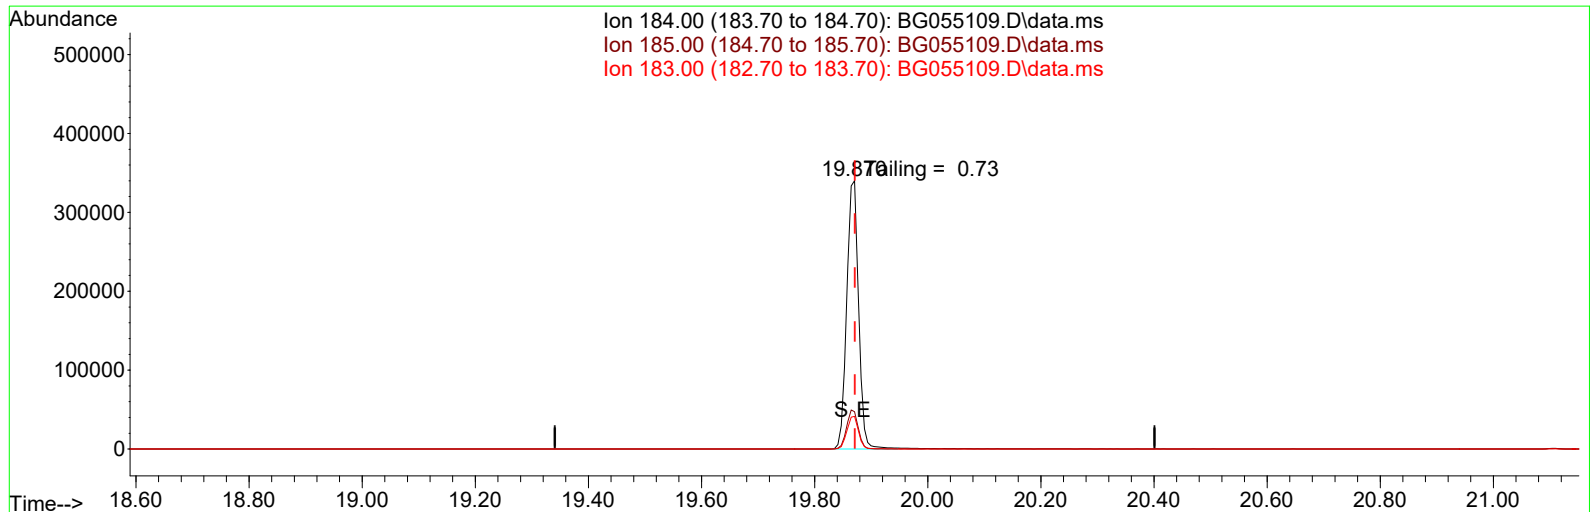

TIC: BG055109.D\data.ms

(77) Benzidine

19.870min (-0.001) 0.00 ng

response 498137

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	13.93
183.00	11.70	12.18
0.00	0.00	0.00