
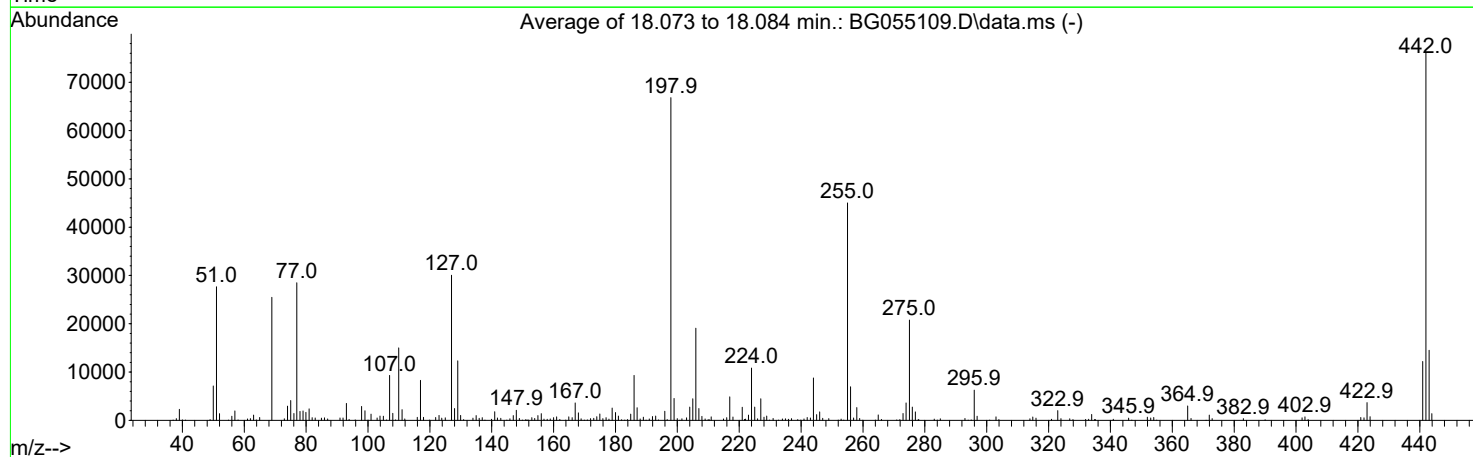


Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101022\
 Data File : BG055109.D
 Acq On : 10 Oct 2022 11:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Oct 08 03:04:59 2022

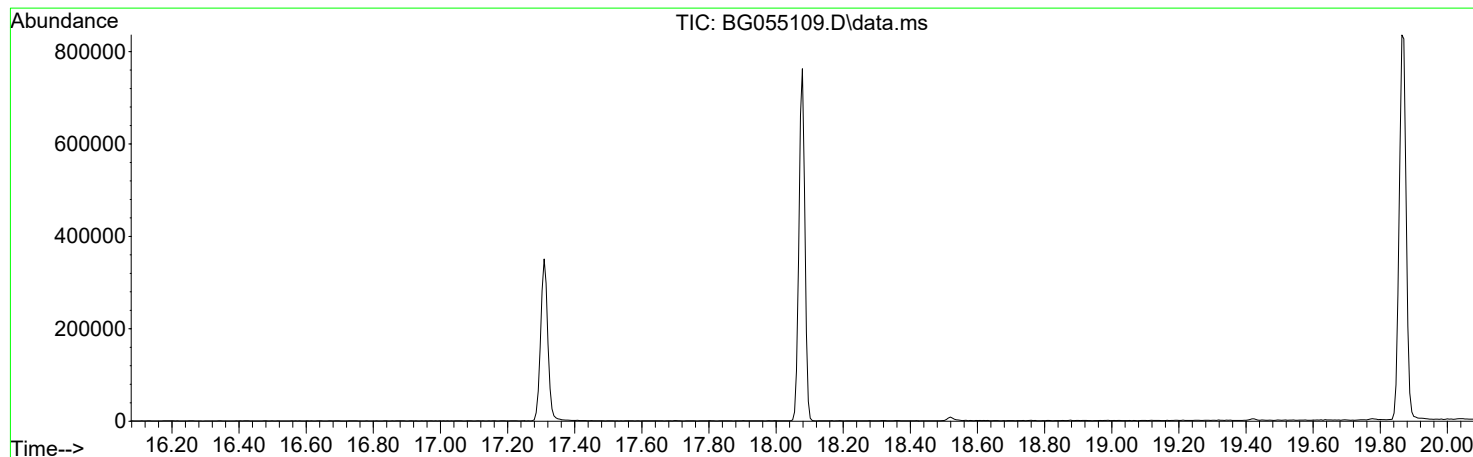




AutoFind: Scans 2516, 2517, 2518; Background Corrected with Scan 2509

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.4	27648	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	38.1	25460	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.9	30035	PASS
197	198	0.00	2	0.2	161	PASS
198	198	100	100	100.0	66835	PASS
199	198	5	9	6.8	4536	PASS
275	198	10	60	31.1	20760	PASS
365	198	1	100	4.5	2987	PASS
441	198	0.01	100	18.2	12184	PASS
442	442	50	100	100.0	76163	PASS
443	442	15	24	19.1	14512	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101022\
Data File : BG055109.D
Acq On : 10 Oct 2022 11:33
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_G
ClientSampleId :
DFTPP

Quant Time: Oct 11 06:15:53 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 08 03:04:59 2022
Response via : Initial Calibration

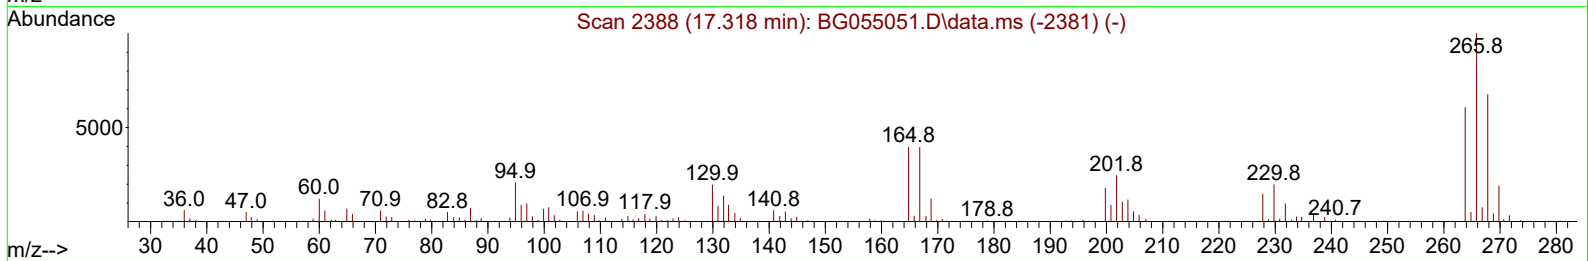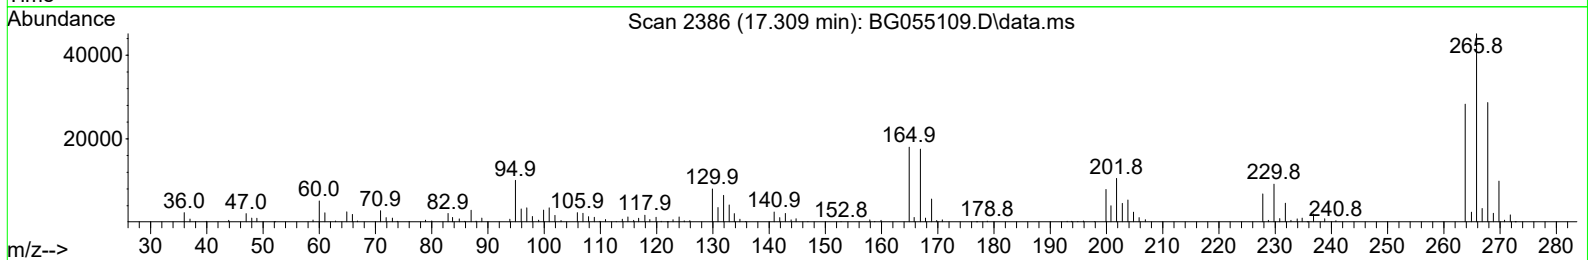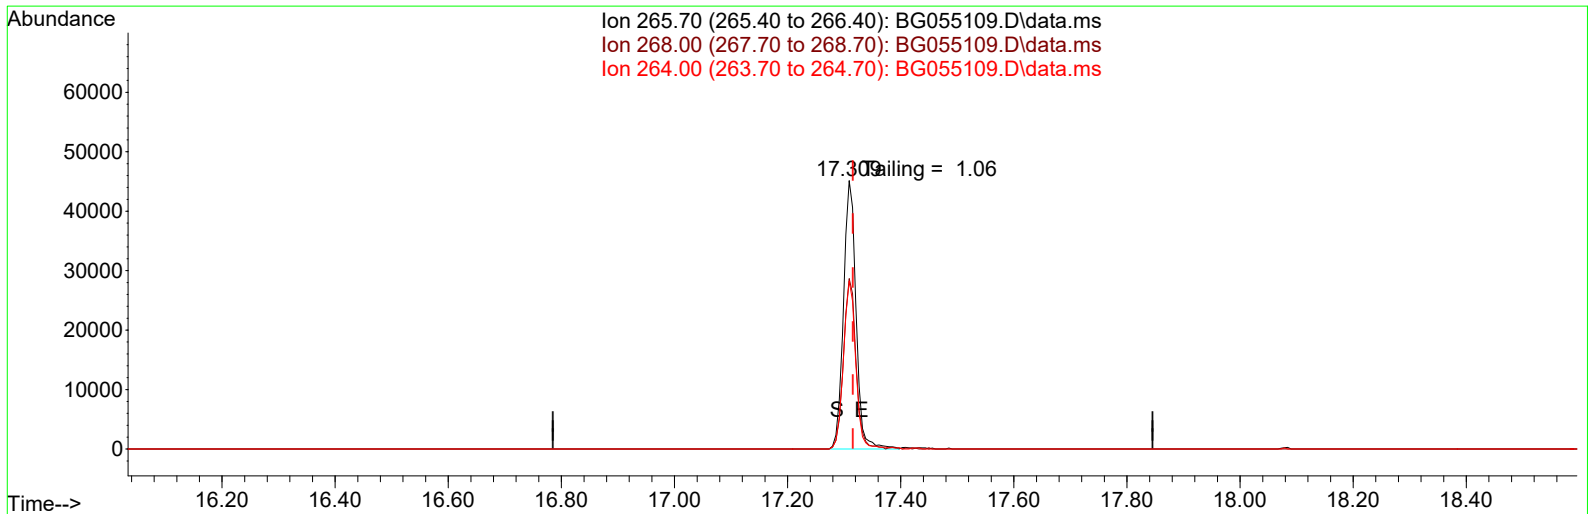

TIC: BG055109.D\data.ms

(70) Pentachlorophenol (C)

17.309min (-0.007) 29399.91 ng




response 69824

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.50	63.53
264.00	60.80	62.66
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_G\Data\BG101022\
 Data File : BG055109.D
 Acq On : 10 Oct 2022 11:33
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_G
 ClientSampleId :
 DFTPP

Quant Time: Oct 11 06:15:53 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_G\Methods\8270-BG100322.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 08 03:04:59 2022
 Response via : Initial Calibration

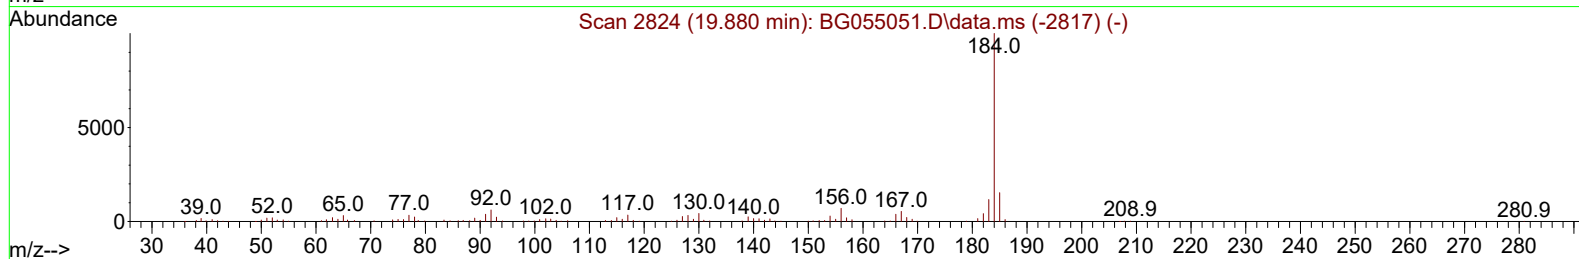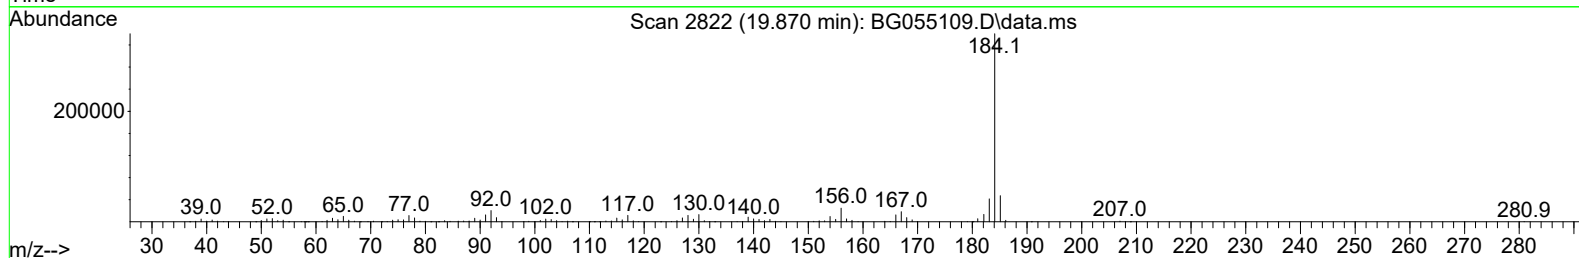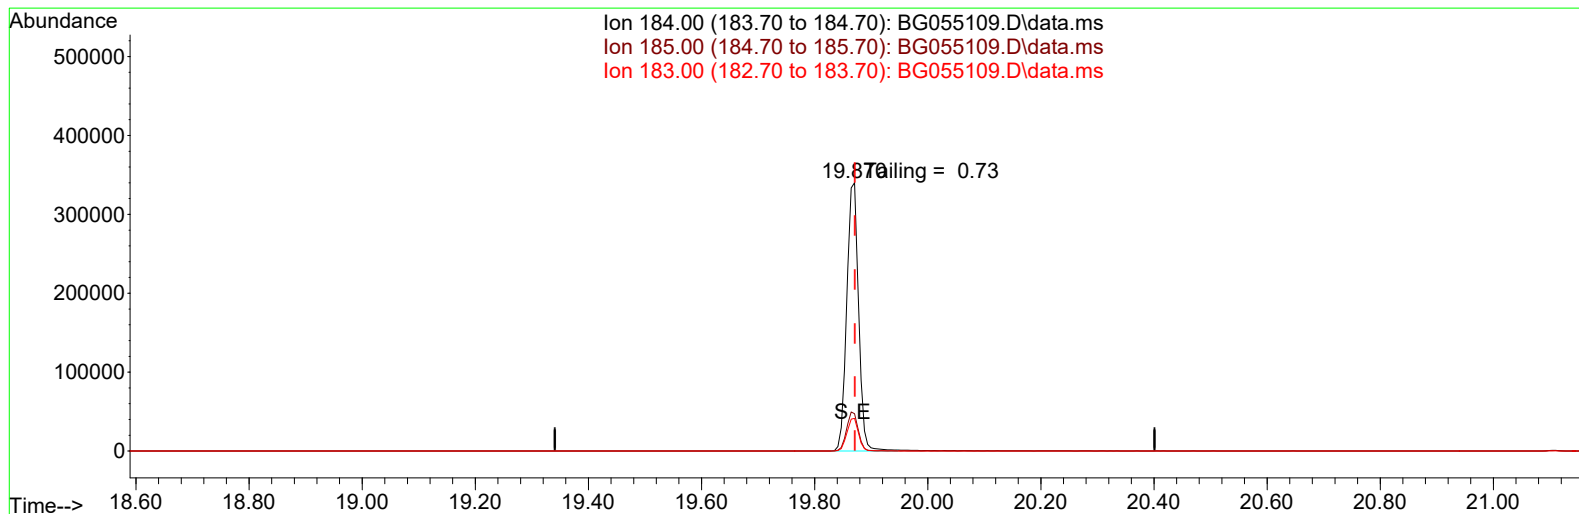

TIC: BG055109.D\data.ms

(77) Benzidine

19.870min (-0.001) 0.00 ng

response 498137

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.30	13.93
183.00	11.70	12.18
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/10/2022	BNA_G	BG055109.D
Compound Name	Response	Retention Time
DDT	192919	21.104
DDD	5214	20.652
DDE	324	20.152
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5538	198457	2.79

Instrument :
BNA_G
ClientSampleId :
DFTPP